

For Healthcare Professionals only

# NObreath<sup>®</sup>

Fractional Exhaled Nitric Oxide (FeNO) Device

## User Manual



CE  
2797

***FeNO testing without limits.***

## Definitions

**WARNING:** Indicates a potentially hazardous situation, which, if not avoided, may result in minor or moderate injury.

**CAUTION:** Indicates a potentially hazardous situation, which, if not avoided, may result in damage to the device.

**NOTE:** Used to call attention to notable information that should be followed during use.

## Important Information/Reminders

**NOTE:** Only technical data and no patient data is collected by Bedfont®.

**NOTE:** The NObreath® should be charged for a minimum of 24 hours before first use.

**NOTE:** The default PIN for the NObreath® is 0000. Bedfont® strongly advises that this PIN is changed upon installation and set-up of the device.

**WARNING:** Please read the manual before use.

**WARNING:** Never use alcohol or cleaning agents containing alcohol or other organic solvents as these vapours will damage the electrochemical sensor inside.

**WARNING:** Under no circumstances should the instrument be immersed or splashed with liquid.

**WARNING:** Breath tests must only be carried out with Bedfont® accessories. Failure to do so may cause incorrect readings.

**WARNING:** The mouthpieces are single patient use only and can be used for a maximum of 10 tests per breath testing session. Further re-use could cause incorrect readings and could increase the risk of cross infection. The mouthpiece should be disposed of after use, in accordance with local waste disposal guidance.

**WARNING:** Patients should exhale for the duration of time indicated by the device during a breath test. Failure to do so may cause incorrect readings.

**WARNING:** To ensure a breath sample is taken at the correct flow rate, the device must be held upright at all times during a breath test.

**WARNING:** Do not block the vent holes on the device at any time. Blocking the vent holes may cause erroneous readings.

**WARNING: Do not allow the use of the NObreath® within 60 minutes of the following:**

- Exercising
- Smoking
- Eating
- Drinking including Alcohol



**WARNING:** Ensure the patient does not inhale through the mouthpiece.

**WARNING:** Ensure the patient does not exhale beyond the limits of their physical ability.

**WARNING:** Ensure the patient uses a single patient use mouthpiece for performing a breath test.

**WARNING:** The USB port is to be used for charging the NObreath® device, this should be carried out via the supplied USB lead and also can be used for transferring encrypted patient data to and from FeNOchart™ PC Software. The NObreath® is not intended to be connected to any wireless adaptors or any other USB Host.

**CAUTION:** Ensure the device is used within the stated operating temperature and humidity ranges. Operating temperature is 15-30°C (59 -86°F). Operating humidity is 20 - 80% RH (non-condensing).

**CAUTION:** Portable and mobile RF communications equipment can affect the NObreath®.

**CAUTION:** A great way to keep the NObreath® charged when not in use is to use the docking station included. This can be connected via the pre-approved mains adapter supplied, or plugged into a working USB port, to ensure the NObreath® has charge for when it's needed. When connecting the pre-approved mains adapter from the docking station to the mains power, please make sure that it is plugged in to a mains location that is safe and easily accessible.

**CAUTION:** The NO scrubber contains potassium permanganate and should not be tampered with or exposed to skin.

**CAUTION:** The NO scrubber contains potassium permanganate and should be disposed of as hazardous waste in accordance with local waste disposal regulations.

**NOTE:** Ensure the patient inhales through the mouth, before exhaling through the mouthpiece.

**NOTE:** Bedfont® advise the NObreath® is charged monthly to ensure calibration data is not lost.

**NOTE:** When selecting an accessory for the NObreath® device, please be advised that an accessory not recommended by Bedfont® may result in loss of performance and damage to the NObreath® device. The product warranty does not cover product failure or damage resulting from use with non-approved accessories.

**NOTE:** See Bedfont's infection control and maintenance guidelines for further information on infection control.

**NOTE:** Please do not attempt to modify the equipment in any way or use accessories not specified by the manufacturer. Any attempt to do so, will invalidate the warranty and may compromise the safety of the device.

**NOTE:** The EMISSIONS characteristics of this equipment make it suitable for use in industrial areas and hospitals (CISPR 11 class A). If it is used in a residential environment (for which CISPR 11 class B is normally required) this equipment might not offer adequate protection to radio-frequency communication services. The user might need to take mitigation measures, such as relocating or re-orienting the equipment.

**NOTE:** Bedfont® will make available on request service training to appropriately qualified personnel.

## Contents

Definitions.....	3
Important Information/Reminders .....	3
Introduction .....	6
Compliance .....	6
Intended Use.....	6
Contraindications .....	6
Parts and accessories.....	7
Instrument Layout.....	8
Installation and Set-up.....	9
User Interface.....	12
Demo mode .....	13
Performing a Breath Test .....	15
Patient Profiles.....	17
Maintenance .....	21
Quality Check .....	22
Calibration using a CaliBag® .....	31
How to carry out a Calibration .....	32
Settings .....	39
Data Reset.....	46
Cybersecurity .....	48
Technical Specification.....	49
Using the NObreath® with FeNOchart™ .....	50
Buttons Explained .....	50
Troubleshooting .....	51
Glossary of Symbols and Safety Information.....	58
Wireless .....	60
Emissions .....	62
Immunity .....	63
Summary of the clinical data .....	65
Warranty.....	68
Vigilance .....	68
Returns .....	68
Responsible Manufacturer and Contacts.....	69

## Introduction

The User Manual provides instructions on how to operate NObreath® FeNO device and its accessories. It contains relevant information about the device, its uses and its care, including step-by-step instructions with screens and illustrations.

## Compliance

NObreath® is CE marked according to the Medical Device Regulation (EU) 2017/745.

NObreath® is RoHS compliant.

Please refer to the 'Safety Information' section of this manual for more information on the compliance of the NObreath®.

## Intended Use

The NObreath® is a portable, non-invasive device for the measurement of Fractional Exhaled Nitric Oxide (FeNO) in human breath. The production of nitric oxide is often found to be increased in inflammatory conditions such as asthma. Measurement of FeNO by NObreath® is a method to measure the decrease in FeNO concentration in asthma patients that often occurs after treatment with anti-inflammatory pharmacological therapy, as an indication of the therapeutic effect in patients with elevated FeNO levels.

The fractional NO concentration in expired breath (FeNO), can be measured by NObreath® according to guidelines for NO measurement established by the American Thoracic Society.

NObreath® is intended for children, 7 - 17 years, and adults 18 years and older. NObreath® 12 second test mode is for age 7 and up.


NObreath® 10 second test mode is for ages 7 - 10 only who cannot successfully complete a 12 second test. FeNO measurements provide the physician with means of evaluating an asthma patient's response to anti-inflammatory therapy, as an adjunct to the established clinical and laboratory assessments in asthma. The NObreath® cannot be used with infants or by children under the age of 7 as measurement requires patient cooperation.

NObreath® should not be used in critical care, emergency care or in anesthesiology.

## Contraindications


There are no known contraindications.

## Parts and accessories

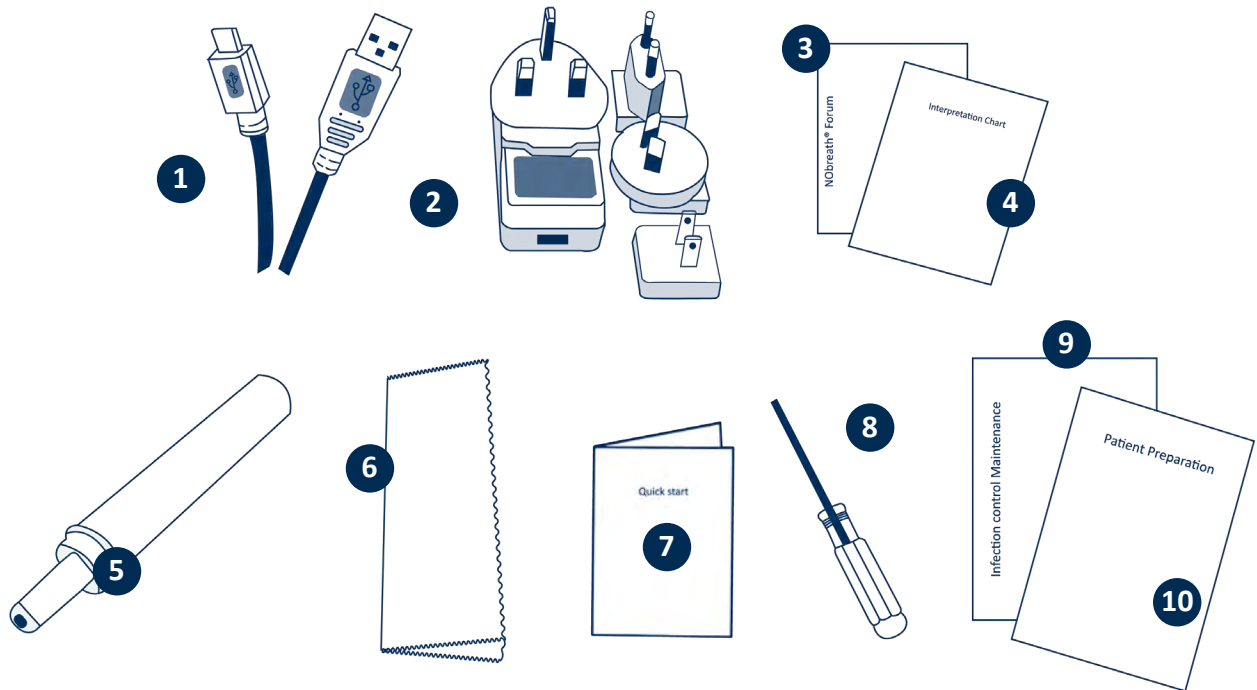

- |    |                                   |     |  |
|----|-----------------------------------|-----|--|
| 1. | 1.8 m USB cable                   | 6.  | Microfiber cloth                         |
| 2. | Mains plug and universal adaptors | 7.  | Quick Start Guide                        |
| 3. | NObreath® Forum information       | 8.  | Screwdriver                              |
| 4. | Interpretation chart              | 9.  | Infection Control Maintenance Guidelines |
| 5. | NObreath® mouthpiece              | 10. | Patient Preparation                      |

## Instrument Layout

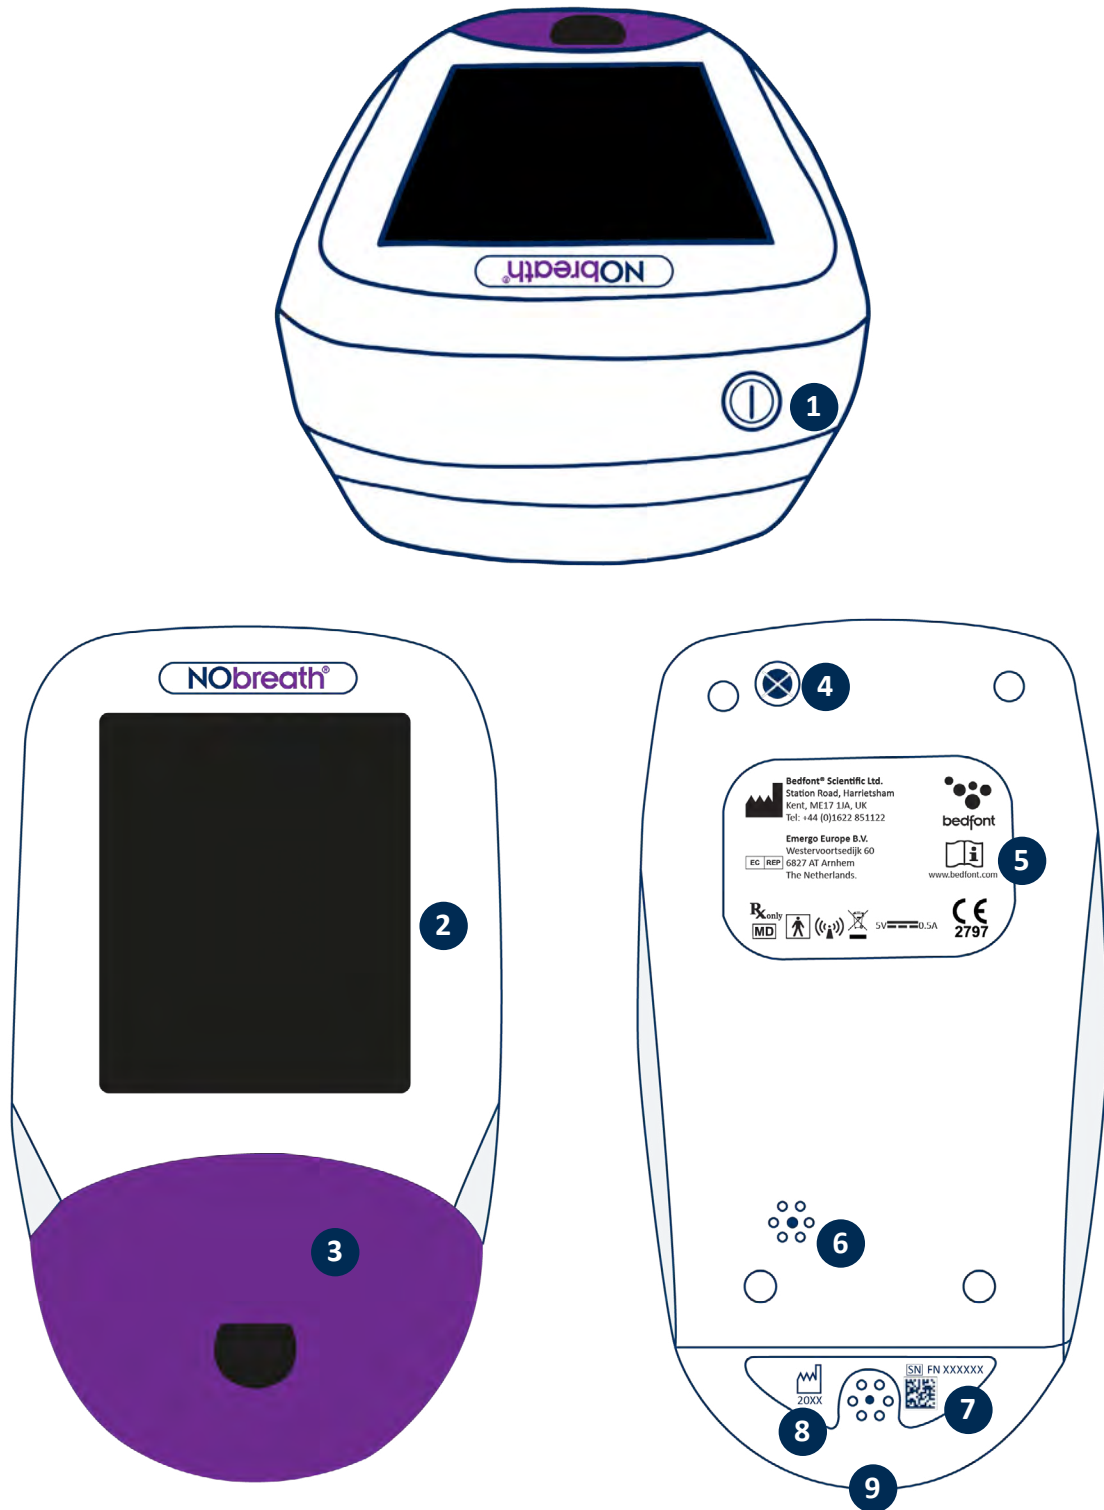

- 1. ON/OFF switch
- 2. Touchscreen
- 3. Mouthpiece aperture
- 4. Screw

- 5. Manufacturer Label
- 6. Vent hole
- 7. Serial label
- 8. Vent hole
- 9. USB port

## Installation and Set-up

When setting up the NObreath<sup>®</sup>, please ensure the package contains all the parts as detailed in the 'Parts and Accessories' section of this manual. Please keep the screwdriver supplied for future servicing requirements. The NObreath<sup>®</sup> should be charged for 24 hours prior to first use. Remove the plastic film from the display and follow the next steps on how to charge the NObreath<sup>®</sup> below.

**NOTE:** *The NObreath<sup>®</sup> should not be operated in an environment outside of the temperature or humidity ranges stated in the technical specification.*

The default PIN is 0000. It is strongly recommended to change this prior to first use – please refer to the 'Change PIN' section of this manual for instructions.

When selecting an accessory for the NObreath<sup>®</sup> device, please be advised that an accessory not recommended by Bedfont<sup>®</sup> may result in loss of performance and damage to the NObreath<sup>®</sup> device. The product warranty does not cover product failure or damage resulting from use with non-approved accessories.

**WARNING:** The mouthpieces are single patient use only and can be used for a maximum of 10 tests per breath testing session. Further re-use could cause incorrect readings and could increase the risk of cross infection. The mouthpiece should be disposed of after use, in accordance with local waste disposal guidance.

### *How to charge the NObreath<sup>®</sup>*

The NObreath<sup>®</sup> FeNO device comes with a Dock (where supplied) and charging cable to keep the device at hand and fully charged.


**NOTE:** *The NObreath<sup>®</sup> should be charged for a minimum of 24 hours before first use.*

**NOTE:** *It is best practice to not let the battery run flat. If the NObreath<sup>®</sup> does not switch on, or displays the battery symbol on the last bar of charge, the NObreath<sup>®</sup> should be charged for 24 hours prior to use.*




The NObreath<sup>®</sup> FeNO device can be charged by plugging the micro USB cable provided directly into the NObreath<sup>®</sup>. This can then be connected either to the pre-approved mains adapter or into a computer USB port.

To charge the NObreath<sup>®</sup>, first make sure the micro USB cable provided is connected to the docking station.

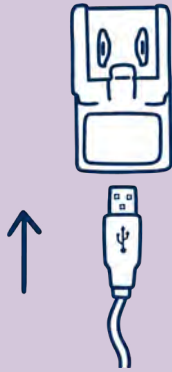


Connect the other end of the micro USB cable to the pre-approved mains adapter supplied, using the appropriate universal adapter.

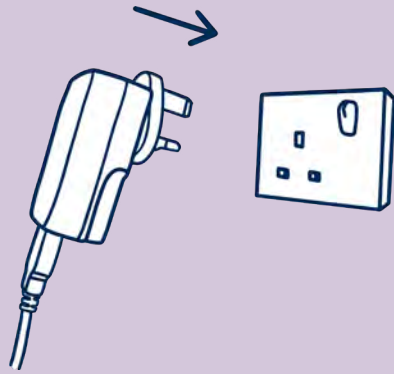

Plug the pre-approved mains plug into the mains power.


*Charging the NObreath using the Docking Station (where supplied)*

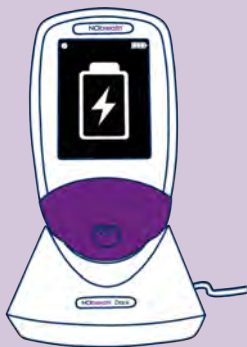

Place the NObreath® device into the Dock. The screen will indicate that the device is charging if powered off.




Connect the other end of the micro USB cable to the pre-approved mains adapter supplied, using the appropriate universal adapter.

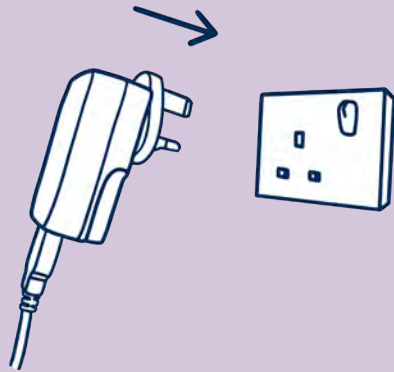


Plug the pre-approved mains adapter into the mains power.

**CAUTION:** When connecting the pre-approved mains adapter from the docking station to the mains power, please make sure that it is plugged in to a mains location that is safe and easily accessible.

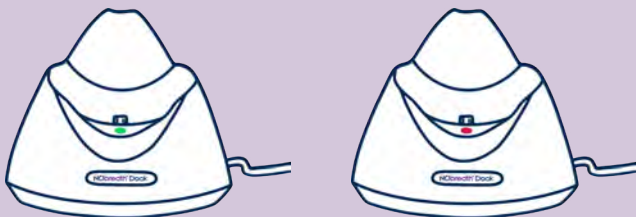

When receiving power, the LED on the Dock will light up green and the NObreath® can be placed in the Dock to charge. If the LED light is red, please see 'Troubleshooting'.


## User Interface

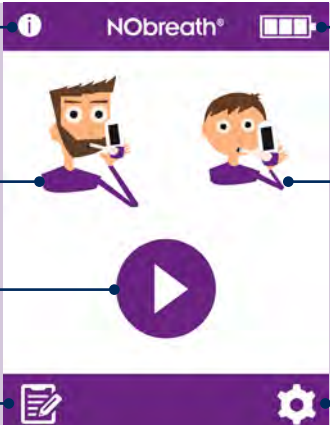

The Home Screen features a purple header with the NObreath logo and battery status. Below the header are two cartoon characters representing an adult and a child, each holding a device. A large play button is centered on the screen. At the bottom, there is a navigation bar with icons for patient profiles and settings.

**Home Screen**

1. Information button.
2. Battery status.
3. Adult breath test.
4. Child breath test.
5. Demo mode.
6. Patient profiles.
7. Settings.




The Information screen displays the following details:

Test No.	1001
Cal date	15/02/2022
Serial No.	NN001232
Sensor date	15/02/2022
Sensor serial No.	157649832
Firmware	VX.XX

A home button is located at the bottom of the screen.


The information screen displays information about the device and sensor.



Settings Menu Page 1 includes options for date and time, test log, PIN settings, flow-meter style, ambient air test, and service area. A home button and a right arrow are also present.

**Settings Menu Page 1**

1. Date and time options.
2. Test log.
3. Change PIN number.
4. Enable/disable PIN use.
5. Change flow-meter style.
6. Start ambient air test.
7. Service Area.
8. Home button.
9. Go to Settings Menu Page 2.

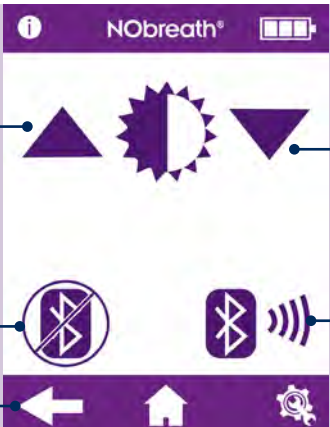


Settings Menu Page 2 includes options for screen brightness, Bluetooth settings, and a back arrow.

**Settings Menu Page 2**

1. Increase screen brightness.
2. Decrease screen brightness.
3. Enable/disable Bluetooth®.
4. Bluetooth® pairing PIN.
5. Go to Settings Menu Page 1.


## Demo mode



The screenshot shows the NObreath app interface. At the top, there is an information icon, the text 'NObreath®', and a battery level indicator. The main area displays two cartoon characters, an adult and a child, each holding a device. Below them is a large purple play button icon. A line with the number '1' points to this play button. At the bottom, there are icons for a document and a settings gear.


1. The NObreath® has an in-built demonstration video of the breath test process. It is recommended to watch this video prior to using the device for the first time. This demo can also be used to explain to patients how the test will run, prior to performing one.

Press the demo icon to begin.




The screenshot shows the NObreath app interface with the two cartoon characters (adult and child) from the previous screen. The play button is no longer visible, indicating that the user has selected a patient type.

Select either the adult or child patient.




The screenshot shows the NObreath app interface with a large hourglass icon in the center, representing the zero screen. The top bar and bottom bar are consistent with the previous screens.

The zero screen will briefly display as in a real test.

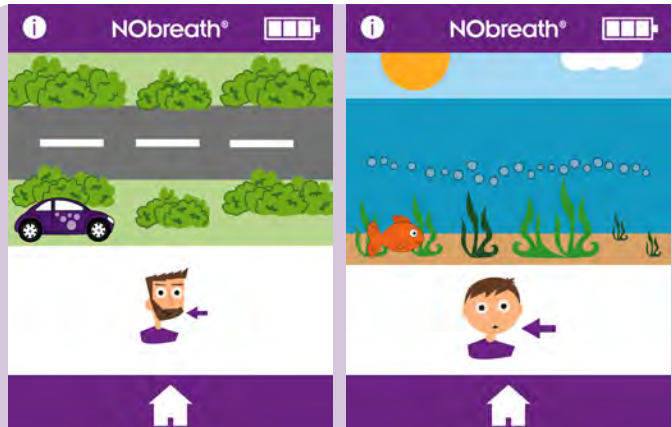

Two side-by-side screenshots of the NObreath app. The left screenshot shows a landscape with trees and a road, with the adult character at the bottom and a blue arrow pointing left. The right screenshot shows an underwater scene with a sun, bubbles, and a fish, with the child character at the bottom and a blue arrow pointing left. Both screenshots have a home icon at the bottom.


A demonstration will run through the breath test process.

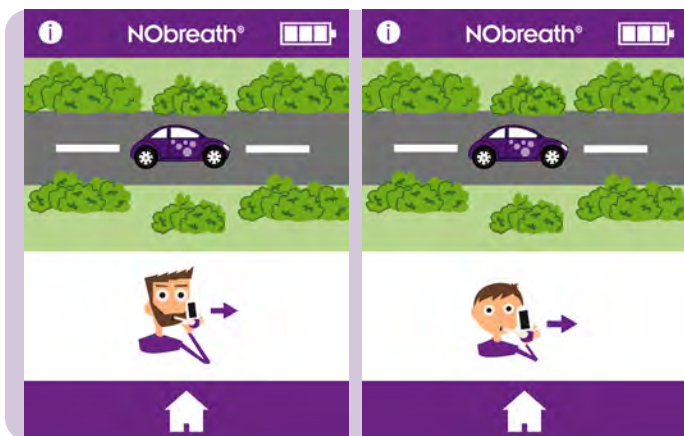

The whole test will be shown, but at an accelerated speed.



Only a successful test will be demonstrated.

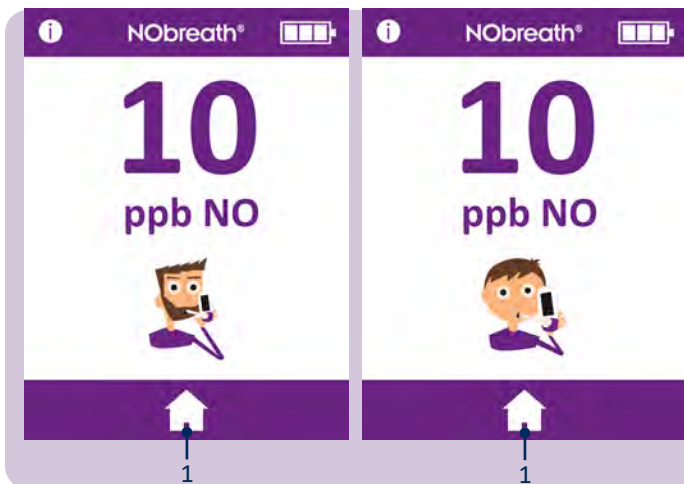

Once the result is displayed, the demo is complete.  
Press the home icon (1) to return to the home screen.

# Performing a Breath Test

1 ————— 2

Open and insert a new mouthpiece into the NObreath® device.

To start a breath test, select either the adult (1) or child (2) patient.

As prompted onscreen, take a deep breath.

**WARNING:** Do not inhale through the mouthpiece.

**NOTE:** Ensure the patient inhales through the mouth, before exhaling through the mouthpiece.

Press the home button at any time to cancel the breath test.

When the exhale icon displays, keep the device upright and blow gently into the mouthpiece.

**NOTE:** Make sure the vent holes are not covered.

The exhalation time is approximately 12 seconds for an adult and 10 for a child.

The onscreen flow meter will guide the patient on the exhalation rate:

Keep the car in the middle of the road.


Keep the dial in the green area.

Keep the car in the middle of the road.

Follow the bubbles.




A green tick onscreen indicates a successful test.

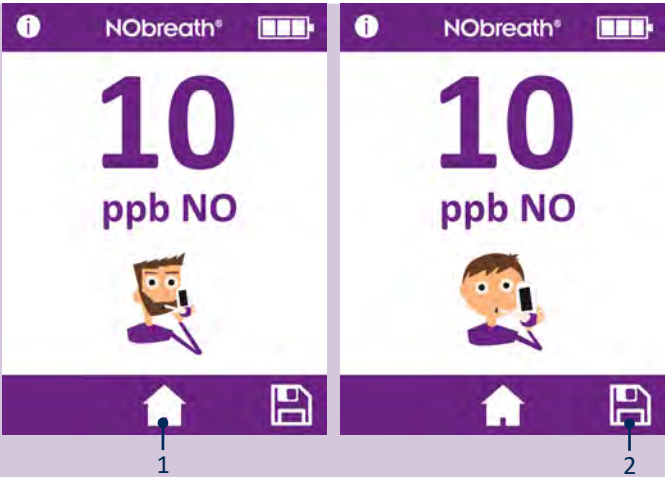

The results will then be shown onscreen in ppb.


Return to the home screen by pressing the home button (1) or save (2) the result to a patient profile.

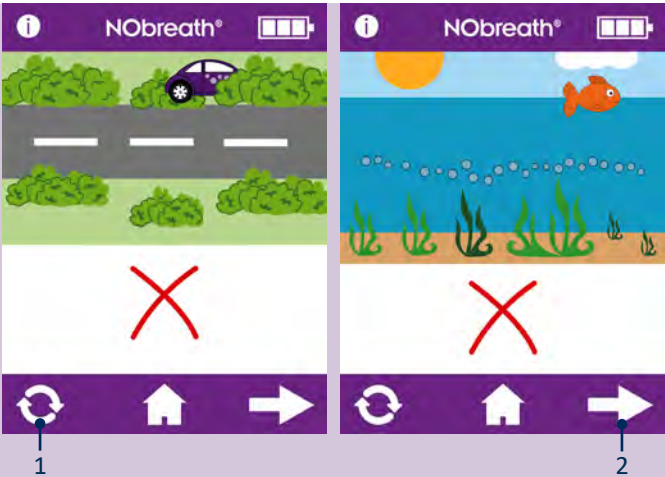

If the patient exhales outside of the exhalation guidelines, the test will beep before indicating a fail and a red cross will appear.

Press the retry icon (1) to retake the test or the next arrow (2) to view the result.

# Patient Profiles

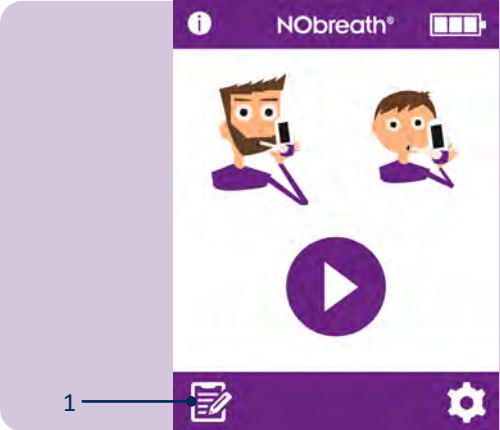

The NObreath® is designed to be capable of storing up to 25 results in up to 50 patient profiles.

Press the profiles icon (1) to access patient profiles.




If the PIN has not been entered in the last 30 minutes, the 4-digit code will be required before the patient profiles can be accessed.

**NOTE:** *If the PIN has been forgotten, please contact Bedfont® or its local distributor to reset it.*




A list of patient profiles will show onscreen.

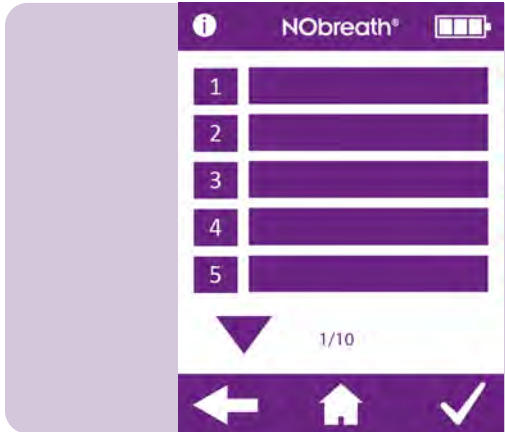

*Create a new patient profile*


To create a new profile, choose an empty name slot.

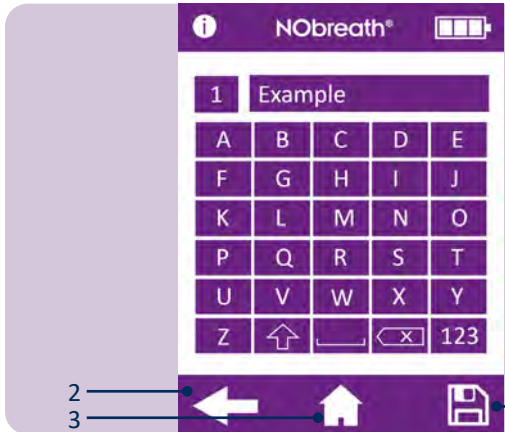

Use the keypad to enter a name or reference.


Click the save icon (1) to create the profile.

To cancel, press the back arrow (2) to return to the list of profiles or the home icon (3) to return to the main screen.

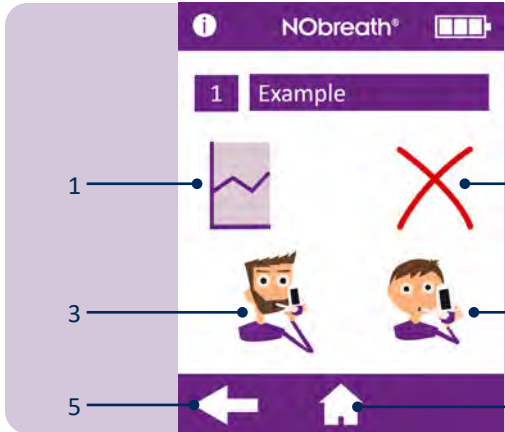


Once the profile has been created the following options will become available:


1. See a graph of results.
2. Delete the patient profile.
3. Take an adult breath test.
4. Take a child breath test.
5. Return to the profile list.
6. Return to the main screen.

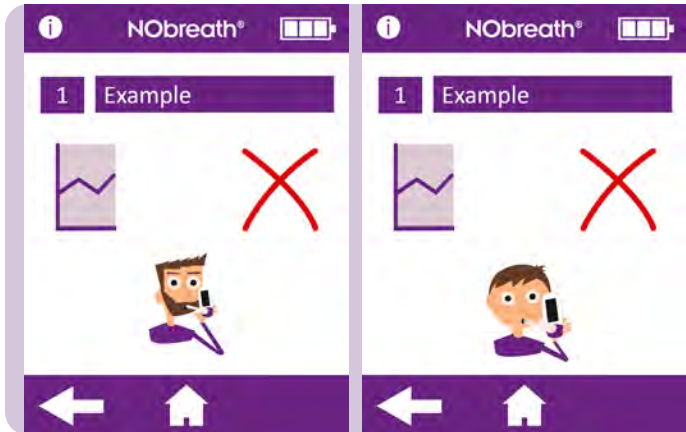

Once an adult or child breath test has been selected, the profile will only offer that breath test mode in future.

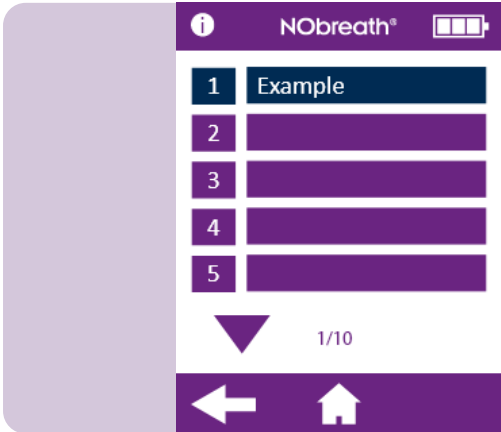


It is not possible for the user to save an adult breath test to a child's profile, or a child's breath test to an adult's profile. Profiles not compatible with the breath test will be shown in blue.

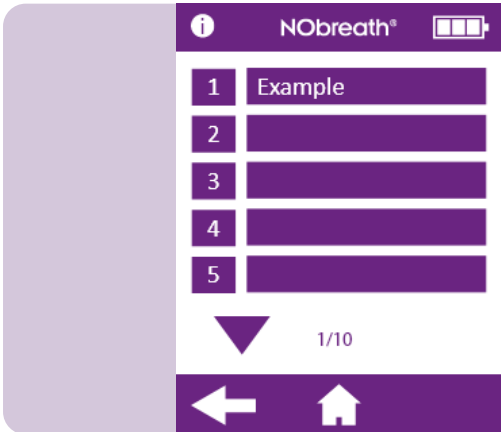


*Edit a new patient profile*

To edit a patient's profile, select their name/ID from the list.

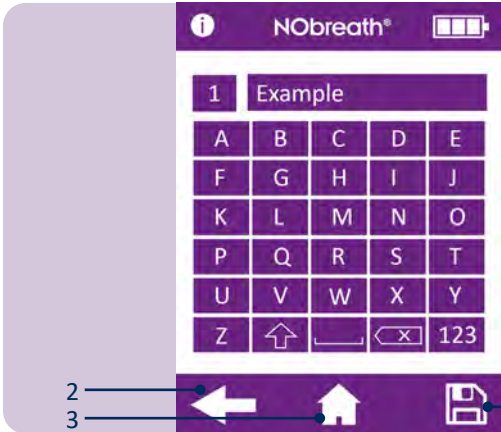


Use the keypad to edit the profile.  
 Click the save icon (1) to save the changes.  
 To cancel, press the back arrow (2) to return to the list of profiles or the home icon (3) to return to the main screen.

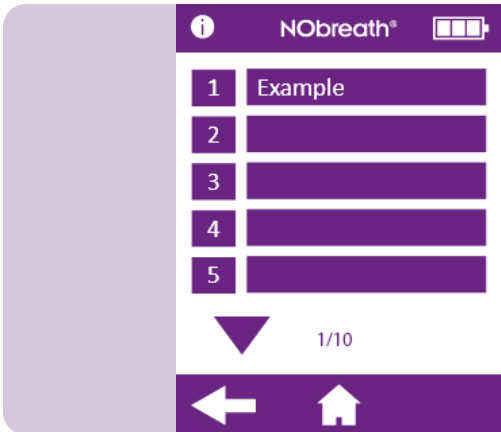


*Delete a patient profile*

Select the patient that will be deleted to load their profile.

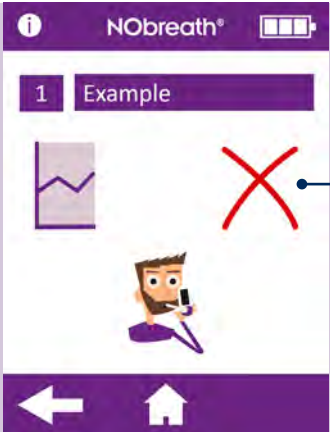

The screenshot shows the NObreath app interface. At the top, there is a status bar with an information icon, the text "NObreath®", and a battery icon. Below this is a header bar with a tab labeled "1" and the text "Example". The main content area contains a line graph icon on the left, a large red "X" icon on the right, and a cartoon character of a man with a beard talking on a mobile phone. At the bottom, there is a navigation bar with a back arrow, a home icon, and a tick mark icon. A blue line with a dot at the end points to the red "X" icon, with the number "1" at the end of the line.

Press the red 'x' (1) to delete the patient profile.

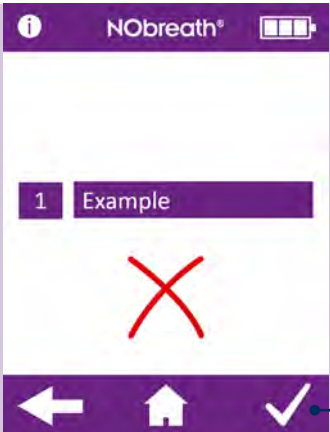


The screenshot shows the NObreath app interface. At the top, there is a status bar with an information icon, the text "NObreath®", and a battery icon. Below this is a header bar with a tab labeled "1" and the text "Example". The main content area contains a large red "X" icon. At the bottom, there is a navigation bar with a back arrow, a home icon, and a tick mark icon. A blue line with a dot at the end points to the tick mark icon, with the number "1" at the end of the line.

Press the tick (1) to confirm.

The profile will be deleted the profile screen will be displayed.

## Maintenance

### NObreath® - FeNO testing without limits

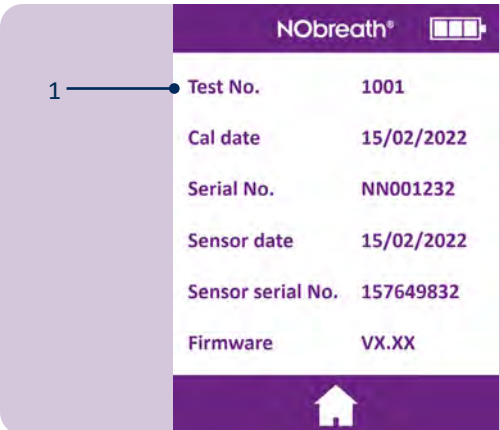

The NObreath® has been validated for up to 29,000 tests when used as instructed and properly maintained and serviced. The number of tests (1) can be periodically checked within the settings of the device; when 29,000 tests are reached a service is recommended. Contact Bedfont® or the local service centre.

The Health Care Professional can check how many breath tests have been performed on the device using the Information Screen, Test No as seen below.

### Routine maintenance

1. Mouthpieces are to be replaced after every patient.


**WARNING:** The mouthpieces are single patient use only and can be used for a maximum of 10 tests per breath testing session. Further re-use could cause incorrect readings and could increase the risk of cross infection. The mouthpiece should be disposed of after use, in accordance with local waste disposal guidance.

2. Hands should be washed regularly in accordance with infection control practice.

**CAUTION:** Do not use sanitising products containing alcohol as this may damage the sensors.

3. Only use accessories approved by Bedfont®.

**CAUTION:** Use of accessories not approved by the manufacturer will invalidate the warranty and may compromise the safety of the device.


4. It is best practice to not let the battery run flat. If the NObreath® indicates the battery level is on the last bar on the display , we recommend charging the device. If the NObreath® battery symbol is flashing on the display, the device would require charging immediately.

5. If the NObreath® battery becomes fully discharged, the device may need calibration. Please contact Bedfont® or its local distributor for advice.

## Quality Check

The NObreath<sup>®</sup> will allow a 2-step quality check to be performed, this should be performed within 6 months before an annual calibration, or more frequently if required. This is to ensure the NObreath<sup>®</sup> is within specification. The 2-step quality check will be carried out using filtered ambient air and 100 ppb Nitric Oxide. Bedfont<sup>®</sup> or the local service center can do this or a Quality Check CaliBag<sup>®</sup> kit can be purchased separately (see Quality Check CaliBag<sup>®</sup> component layout below).

This kit contains:

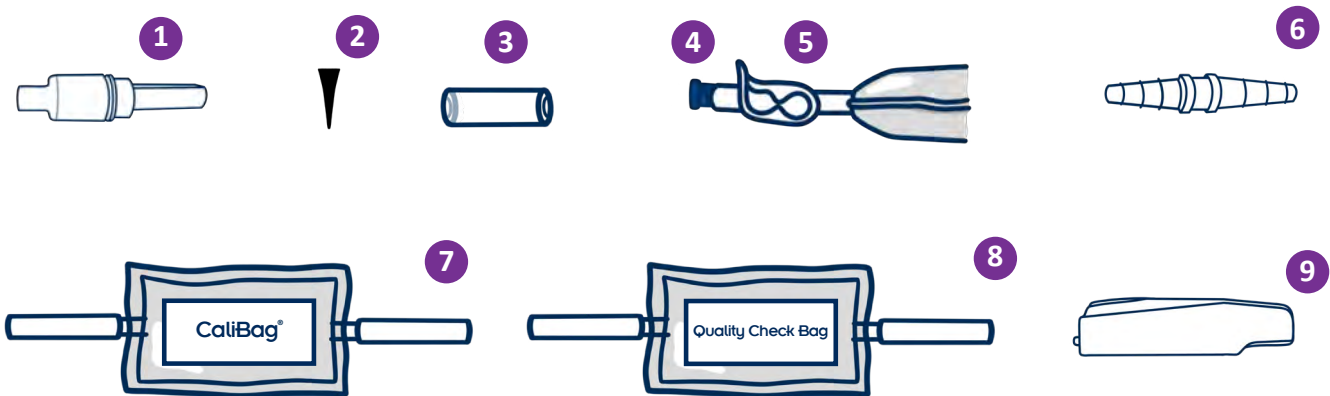

1) CaliAdapter x1

2) Bung x1

3) Scrubber Adapter x1

4) Blue Plugs x2

5) Bag Clamps x2


6) Bag Adapter x1

7) CaliBag<sup>®</sup> x1


8) Quality Check Bag x1

9) NO Scrubber x1


### How to carry out a Quality Check for 0 ppb

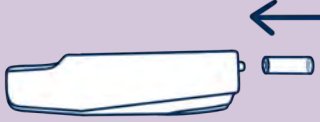

Attach the Scrubber Adapter to the Scrubber.  
**CAUTION:** NO scrubber contains potassium permanganate and should not be tampered with and should not be exposed to skin.




Next, attach the scrubber to the CaliAdapter.

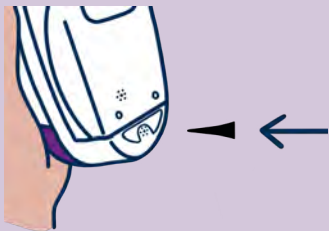


Insert the Bung into the bottom vent hole on the back of the NObreath®.



Turn on the NObreath®.

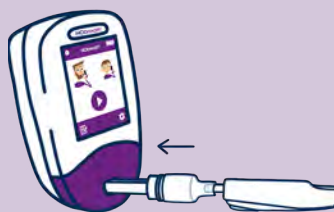

Insert the other end of the CaliAdapter into the NObreath®.

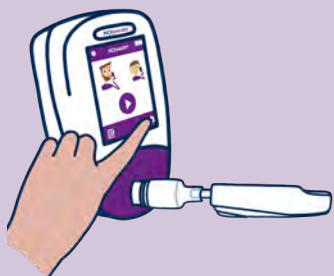

Press the Settings icon.



Press the Ambient Test icon.




An hourglass will appear onscreen while the NObreath® performs the Quality Check without gas.




A reading will appear onscreen; a successful Quality Check will display an NO reading  $\leq 5$  ppb.



If the NO reading is  $> 5$  ppb, please follow the next steps on replacing the NO scrubber and performing a Quality Check with gas.

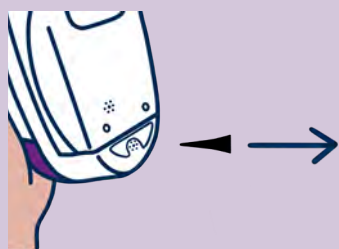

Remove the Bung from the NObreath®.

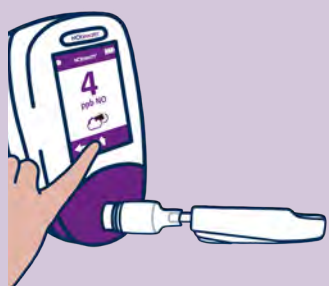

Press the Home icon to return to the home screen.

### *How to replace the NO Scrubber*




Please ensure the NObreath® device is switched off before removing the back cover.



Using the screwdriver provided with the NObreath®, unscrew the screw on the back of the device.



Remove the back cover by sliding and lifting it off.

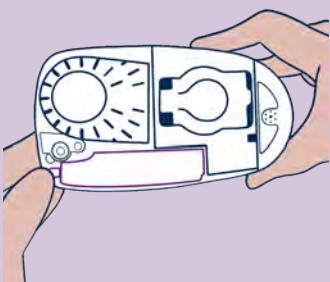

To remove the scrubber, first press down on clip at the top left-hand side of the device.



Slide out the scrubber then lift to remove.  
**CAUTION:** NO scrubber contains potassium permanganate and should be disposed of as hazardous waste in accordance with local waste disposal regulations.



Using the same NO Scrubber from the Quality Check without gas, insert this into the NObreath®. Please ensure the CaliAdapter and Scrubber Adapter have been removed from the scrubber before inserting into the NObreath®.




Re-attach the back cover of the NObreath® device.




To secure the NObreath® back cover in place, use the screwdriver to rescrew the screw into place.


*How to carry out a Quality Check with Gas*




Attach the Bag Adapter to the rubber end of the CaliAdapter.

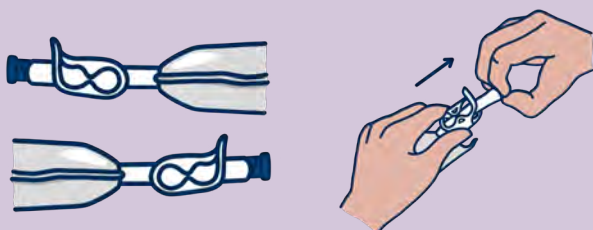

Ensure both Bag Clamps on the Quality Check Bag are closed and remove a Blue Plug from one end.  
NOTE: Make sure the Quality Check Bag is being used.




Insert the Bag Adapter into the Quality Check Bag.

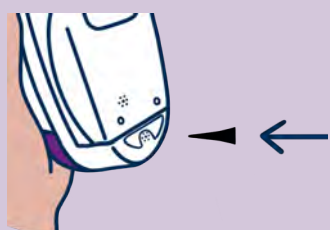


Insert the Bung into the bottom vent hole on the back of the NObreath®.




Turn on the NObreath®.

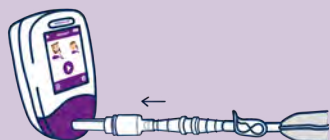


With the Quality Check Bag attached, insert the CaliAdapter into the NObreath®.

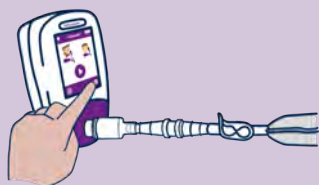


Press the Settings icon.

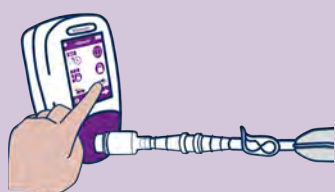


Press the Ambient Test icon.




When an hourglass appears, open the clamp while the NObreath® performs the Quality Check with gas. The device will automatically draw gas from the Quality Check Bag.

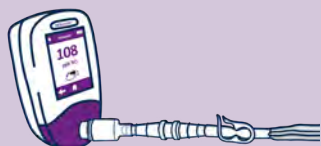


A reading will appear on-screen; a successful Quality Check will display an NO reading within  $\pm 10\%$  of the gas concentration written on the Quality Check Bag label. For guidance please refer to the Quality Check conversion chart which can be found in the Quick Start Guide.

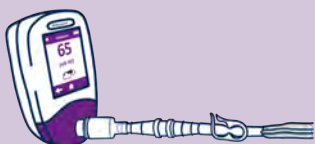

If the NO reading is not within  $\pm 10\%$  of the concentration written on the Quality Check Bag label, the NObreath® requires a calibration. To calibrate the device with the CaliBag®, follow the instructions provided.



Ensure both Bag Clamps are closed before removing the Quality Check Bag and all adapters from the NObreath®.

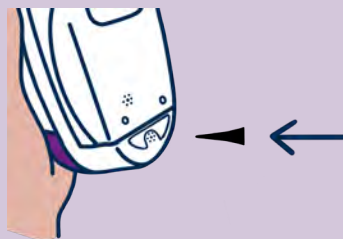

Remove the Bung from the NObreath®.



Press the Home icon to return to the home screen.

**If the reading is not within the specification of the concentration range, one of the following should be carried out:**

1. Calibrate using a CaliBag®.
2. Send the device back to Bedfont® or local service center for investigation.
3. Replace with a pre-calibrated sensor; Bedfont® or the local service center can do this for or a sensor replacement kit can be purchased separately which is supplied with replacement instructions.


### Calibration using a CaliBag®

**NOTE:** The device must be calibrated annually at the following temperature of  $21^{\circ}\text{C} \pm 4^{\circ}\text{C}$  ( $70^{\circ}\text{F} \pm 7^{\circ}\text{F}$ ) or  $70^{\circ}\text{F} \pm 7^{\circ}\text{F}$  ( $63^{\circ}\text{F} - 77^{\circ}\text{F}$ ).


The device will indicate whether the temperature range is out of specification by the following.

	Device too cold to be calibrated	Leave device in an atmospheric temperature of $21^{\circ}\text{C} \pm 4^{\circ}\text{C}$ ( $70^{\circ}\text{F} \pm 7^{\circ}\text{F}$ ) until the temperature range within the device has equilibrated.
	Device too hot to be calibrated	Leave device in an atmospheric temperature of $21^{\circ}\text{C} \pm 4^{\circ}\text{C}$ ( $70^{\circ}\text{F} \pm 7^{\circ}\text{F}$ ) until the temperature range within the device has equilibrated.


## How to carry out a Calibration




Attach the Bag Adapter to the rubber end of the CaliAdapter.

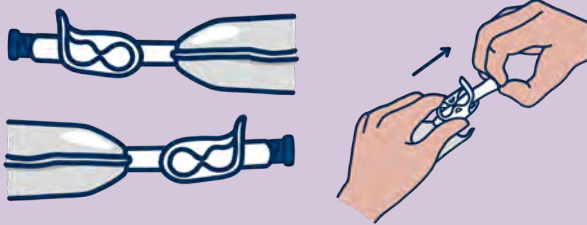


Ensure both Bag Clamps on the CaliBag® are closed and remove a Blue Plug from one end.



Insert the Bag Adapter into the CaliBag®.

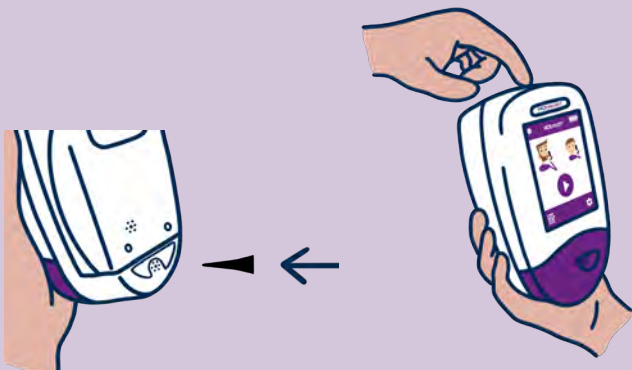

Insert the Bung into the bottom vent hole on the back of the NObreath® and turn the device on.

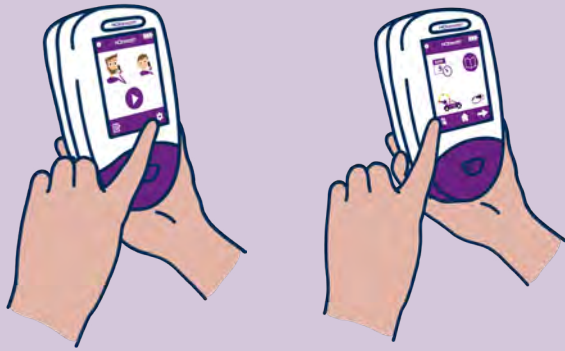


Press the Settings icon, followed by the Service Area icon.



Press the Calibration icon to begin.




Use the arrows to adjust the NO concentration on-screen to match the value of the NO concentration written on the CaliBag®. Press the arrow icon twice to continue

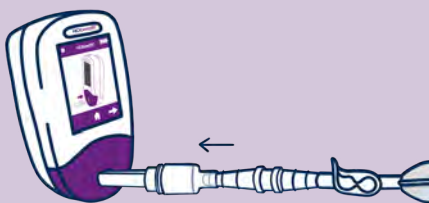


With the CaliBag® attached, insert the CaliAdapter into the NObreath®. Press the next arrow once to continue.


**NOTE:** Make sure the calibration gas CaliBag® is being used.

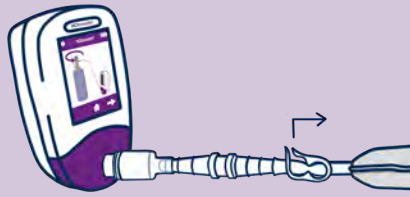


Open the Bag Clamp and press the next arrow to continue.

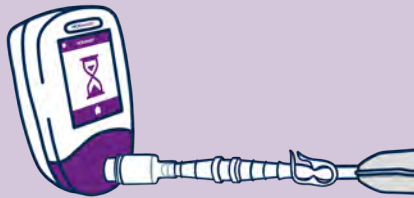


An hourglass will display on-screen as the device will automatically calibrate, drawing the gas from the CaliBag®.

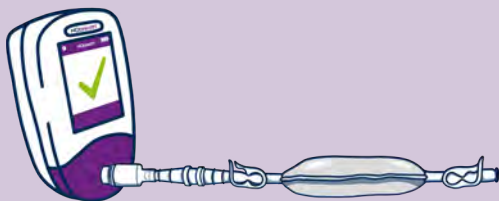


A successful calibration is shown by a green tick. Press save to complete the calibration.

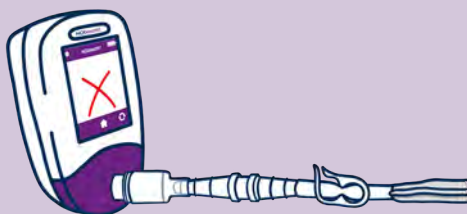

An unsuccessful calibration is shown by a red cross. Press the Retry icon and repeat steps to reattempt the calibration. If the problem persists, please contact Bedfont® or the local distributor.



Ensure both Bag Clamps are closed before removing the CaliBag® and remove all adapters from the NObreath®.

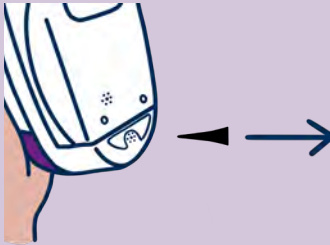





Remove the Bung from the NObreath®.

### Servicing

1. The NObreath® will allow a 2-step quality check to be performed as frequently as the guidelines require between annual services; this is to ensure the NObreath® is within specification. The 2-step quality check will be carried out using filtered ambient air and 100 ppb Nitric Oxide. Alternatively the unit can be sent back to Bedfont® or local service provider.
2. The NO scrubber should be replaced annually and is included in the CaliBag® kit.
3. We recommend the NO sensor, breath drying cartridge and the pump are replaced every 5 years; Bedfont® or local service center can do this.

Do not attempt to open the NObreath® device to gain access to hidden interior components. The back cover is provided to allow safe access to specified removable components, as directed in this manual.

 <p>Firmware v3.53</p>	 <p>Firmware v4.02 and above</p>	<table border="1"> <thead> <tr> <th data-bbox="799 284 999 389"><i>Possible Cause</i></th> <th data-bbox="999 284 1492 389"><i>Recommended Action</i></th> </tr> </thead> <tbody> <tr> <td data-bbox="799 389 999 833"> <p>The sensor requires calibrating or changing and the NO scrubber requires replacing within <math>\leq 30</math> days.</p> </td> <td data-bbox="999 389 1492 833"> <p>The calibration or change of the sensor and the replacement of the NO scrubber is due by the date displayed onscreen.</p> <p>This reminder will be displayed every day until it has been reset by performing a sensor calibration or sensor change, and the NO scrubber has been replaced.</p> </td> </tr> </tbody> </table>	<i>Possible Cause</i>	<i>Recommended Action</i>	<p>The sensor requires calibrating or changing and the NO scrubber requires replacing within <math>\leq 30</math> days.</p>	<p>The calibration or change of the sensor and the replacement of the NO scrubber is due by the date displayed onscreen.</p> <p>This reminder will be displayed every day until it has been reset by performing a sensor calibration or sensor change, and the NO scrubber has been replaced.</p>
<i>Possible Cause</i>	<i>Recommended Action</i>					
<p>The sensor requires calibrating or changing and the NO scrubber requires replacing within <math>\leq 30</math> days.</p>	<p>The calibration or change of the sensor and the replacement of the NO scrubber is due by the date displayed onscreen.</p> <p>This reminder will be displayed every day until it has been reset by performing a sensor calibration or sensor change, and the NO scrubber has been replaced.</p>					

 <p>Firmware v3.53</p>	 <p>Firmware v4.02 and above</p>	<table border="1"> <thead> <tr> <th data-bbox="799 936 999 1041"><i>Possible Cause</i></th> <th data-bbox="999 936 1492 1041"><i>Recommended Action</i></th> </tr> </thead> <tbody> <tr> <td data-bbox="799 1041 999 1480"> <p>The calibration or changing of the sensor and replacement of the NO scrubber is now due.</p> </td> <td data-bbox="999 1041 1492 1480"> <p>The calibration or change of the sensor and the replacement of the NO scrubber is due by the date displayed onscreen.</p> <p>This reminder will be displayed every day until it has been reset by performing a sensor calibration or sensor change, and the NO scrubber has been replaced.</p> </td> </tr> </tbody> </table>	<i>Possible Cause</i>	<i>Recommended Action</i>	<p>The calibration or changing of the sensor and replacement of the NO scrubber is now due.</p>	<p>The calibration or change of the sensor and the replacement of the NO scrubber is due by the date displayed onscreen.</p> <p>This reminder will be displayed every day until it has been reset by performing a sensor calibration or sensor change, and the NO scrubber has been replaced.</p>
<i>Possible Cause</i>	<i>Recommended Action</i>					
<p>The calibration or changing of the sensor and replacement of the NO scrubber is now due.</p>	<p>The calibration or change of the sensor and the replacement of the NO scrubber is due by the date displayed onscreen.</p> <p>This reminder will be displayed every day until it has been reset by performing a sensor calibration or sensor change, and the NO scrubber has been replaced.</p>					



Firmware v4.02 and above

Possible Cause	Recommended Action
<p>The calibration or changing of the sensor and replacement of the NO scrubber is now overdue by <math>\geq 30</math> days.</p> <p>The date displayed is 365 days after the last sensor calibration or exchange.</p>	<p>The calibration or changing of the sensor and replacement of the NO scrubber was due on the date displayed.</p> <p>This reminder will be displayed every day until it has been reset by performing a sensor calibration or sensor change, and the NO scrubber has been replaced.</p>



Firmware v3.53



Firmware v4.02 and above

Possible Cause	Recommended Action
<p>The NObreath<sup>®</sup> is due its full service in <math>\leq 30</math> days.</p>	<p>The NObreath<sup>®</sup> is due its full service by the date displayed.</p> <p>A service reminder will be displayed every day until a full service has been carried out by a trained engineer.</p>



Firmware v3.53



Firmware v4.02 and above

Possible Cause	Recommended Action
<p>The NObreath<sup>®</sup> is now due its full service.</p> <p>5 years has elapsed since last full service.</p>	<p>The NObreath<sup>®</sup> was due its full service on the date displayed.</p> <p>A service reminder will be displayed every day until a full service has been carried out by a trained engineer.</p>

		<table border="1"> <thead> <tr> <th data-bbox="799 284 997 387"><i>Possible Cause</i></th> <th data-bbox="997 284 1497 387"><i>Recommended Action</i></th> </tr> </thead> <tbody> <tr> <td data-bbox="799 387 997 833">The full service for the NObreath® is now overdue by ≥ 30 days.</td> <td data-bbox="997 387 1497 833">The full service for the NObreath® was due on the date displayed. A service reminder will be displayed every day until a full service has been carried out by a trained engineer.</td> </tr> </tbody> </table>	<i>Possible Cause</i>	<i>Recommended Action</i>	The full service for the NObreath® is now overdue by ≥ 30 days.	The full service for the NObreath® was due on the date displayed. A service reminder will be displayed every day until a full service has been carried out by a trained engineer.
<i>Possible Cause</i>	<i>Recommended Action</i>					
The full service for the NObreath® is now overdue by ≥ 30 days.	The full service for the NObreath® was due on the date displayed. A service reminder will be displayed every day until a full service has been carried out by a trained engineer.					

	<table border="1"> <thead> <tr> <th data-bbox="799 934 997 1037"><i>Possible Cause</i></th> <th data-bbox="997 934 1497 1037"><i>Recommended Action</i></th> </tr> </thead> <tbody> <tr> <td data-bbox="799 1037 997 1482">The sensor is stabilising after installation. The time displayed shows the time remaining until sensor is stabilised.</td> <td data-bbox="997 1037 1497 1482">The sensor requires 24 hours to stabilise; during this period, the NObreath® should be placed on charge. During this period, testing will not be possible. This screen will clear automatically after 24 hours.</td> </tr> </tbody> </table>	<i>Possible Cause</i>	<i>Recommended Action</i>	The sensor is stabilising after installation. The time displayed shows the time remaining until sensor is stabilised.	The sensor requires 24 hours to stabilise; during this period, the NObreath® should be placed on charge. During this period, testing will not be possible. This screen will clear automatically after 24 hours.
<i>Possible Cause</i>	<i>Recommended Action</i>				
The sensor is stabilising after installation. The time displayed shows the time remaining until sensor is stabilised.	The sensor requires 24 hours to stabilise; during this period, the NObreath® should be placed on charge. During this period, testing will not be possible. This screen will clear automatically after 24 hours.				

*Cleaning*

Bedfont® recommends wiping the instrument external surfaces between each patient with an alcohol-free wipe specifically designed for this purpose. A list of approved wipes can be found here: <https://www.bedfont.com/cleaning-bedfont-devices>


The device or consumables cannot be sterilised. It is recommended that wipes are used once and for one surface only. The NObreath® device should be cleaned for initial use and after each patient use.

**CAUTION:** Do not use any substances containing alcohol on or near the NObreath®.

**WARNING:** Under no circumstances should the instrument be immersed or splashed with liquid.


**NOTE:** Circuit diagrams, component part lists, descriptions, and calibration instructions can be found in the NObreath® Service Manual. Please contact the local distributor to obtain a copy.

# Settings

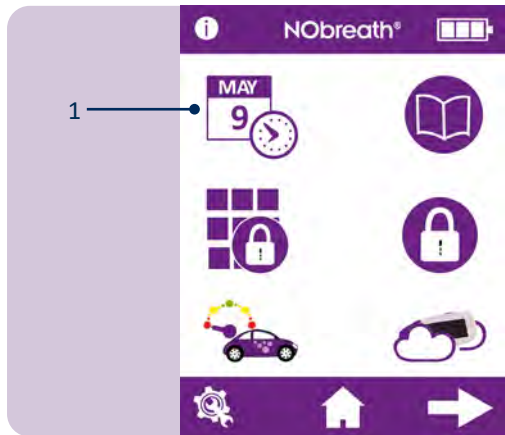

## Settings

To change the date or time, press the edit date/time icon (1) on the 1st page of the settings menu.

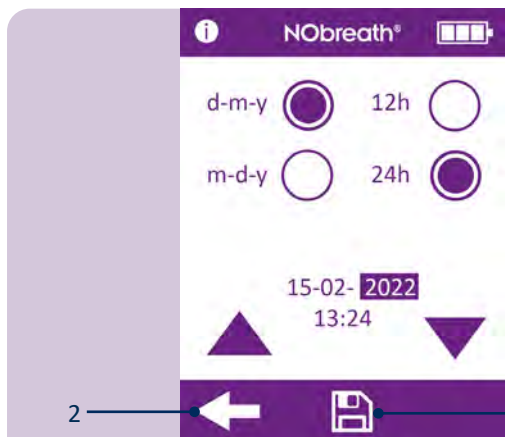

Select either d-m-y or m-d-y for the date format and 12h or 24h for the time format. The purple circle  indicates the selected option.

To adjust the date/time, select the number and it will become highlighted. Use the arrows to change as desired.


Press the save button (1) to keep the changes.

To cancel, press the back arrow (2) to return to the settings menu.



## Test log

To access the test log, press the log icon (1) on the 1st page of the settings menu.




	Date	Time	Reading
1	15/02/2022	15:58	4 ppb
2	15/02/2022	15:57	7 ppb
3	15/02/2022	15:57	33 ppb
4	15/02/2022	15:46	5 ppb
5	15/02/2022	15:45	3 ppb
6	15/02/2022	15:45	0 ppb
7	15/02/2022	15:44	40 ppb

1 points to the down arrow, 1 to the up arrow, 2 to the left arrow, and 3 to the home icon.

The most recent test results are automatically saved in the log and the NObreath® can store 250 at a time.

Use the arrows (1) to scroll through the log.

Press the back arrow (2) to return to the settings menu or the home icon (3) to return to the main screen.




1 points to the change PIN icon.

### Change PIN

Each device is pre-set to the PIN code 0000. It is highly recommended that the PIN is changed to a memorable 4-digit number.

To change the PIN number, press the change PIN icon (1) from the 1st page of the settings menu.



PIN Number

— — — —


0 1 2 3 4

5 6 7 8 9

← Home →

A prompt will ask for the current PIN to be entered.

If the PIN has been forgotten, please contact Bedfont® or its local distributor to reset it.

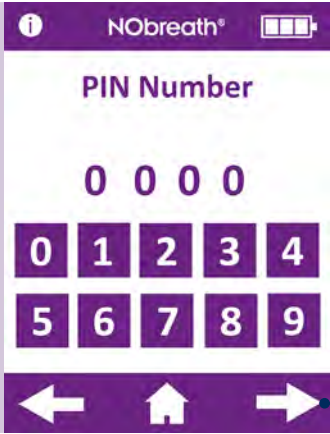

PIN Number

0 0 0 0

0 1 2 3 4

5 6 7 8 9


← Home →

1 points to the right arrow.


Enter the current PIN and press the next arrow (1) to proceed.




A prompt will then ask for a new PIN number to be entered.



Enter a new memorable 4-digit code and press the next arrow (1) to continue.



A prompt will ask for the new PIN number to be re-entered for confirmation.



Re-enter the PIN to confirm the new 4-digit code and press the tick (1) to register the change.

To cancel, press the back arrow (2) to return to the settings menu or the home icon (3) to return to the main screen.

### Enable/disable PIN

To disable the PIN, press the enable/disable PIN icon (1) on the 1st page of the settings menu.



A prompt will ask for the PIN number to be entered in order to disable the PIN function.



Once the PIN function is disabled, it will be crossed out in the settings menu.


To re-enable the PIN function, simply press the enable/disable button again and re-enter the PIN to confirm.



### Change flow-meter style


To change the flow-meter style, press the flow-meter button (1) on the 1st page of the settings menu.






The screenshot shows the NObreath app settings screen. At the top, there is an information icon, the text "NObreath®", and a battery icon. Below this, there are two large rounded rectangular buttons. The left button features an illustration of an adult man with a beard using a spirometer. The right button features an illustration of a child using a spirometer. Below these buttons, there are two smaller icons: a colorful flow-meter and a fish. At the bottom of the screen, there is a navigation bar with a left-pointing arrow and a home icon.

Select either the adult or child test mode to change the flow-meter style.




The screenshot shows the NObreath app settings screen. At the top, there is an information icon, the text "NObreath®", and a battery icon. Below this, there are two car icons: a purple one on the left and a red one on the right. Below the cars, there are two icons: a colorful flow-meter and a fish. The flow-meter icon is highlighted with a white border. At the bottom of the screen, there is a navigation bar with a save icon (a floppy disk).

The current flow-meter style will be highlighted.



The screenshot shows the NObreath app settings screen. At the top, there is an information icon, the text "NObreath®", and a battery icon. Below this, there are two car icons: a purple one on the left and a red one on the right. Below the cars, there are two icons: a colorful flow-meter and a fish. The red car icon is highlighted with a white border. At the bottom of the screen, there is a navigation bar with a save icon (a floppy disk). A line with the number "1" points to the save icon.

Select the new style and press the save icon (1) to register.




The screenshot shows the NObreath app settings screen. At the top, there is an information icon, the text "NObreath®", and a battery icon. Below this, there are two large rounded rectangular buttons. The left button features an illustration of an adult man with a beard using a spirometer. The right button features an illustration of a child using a spirometer. Below these buttons, there are two smaller icons: a red car and a fish. At the bottom of the screen, there is a navigation bar with a left-pointing arrow and a home icon. A line with the number "1" points to the left-pointing arrow, and a line with the number "2" points to the home icon.

The new flow-meter style will now be used for that breath test mode and the relevant demo mode.

Press the back arrow (1) to return to the settings menu or the home icon (2) to return to the main screen.

### Ambient air test

To perform an ambient air test, press the ambient test icon (1) on the 1st page of the settings menu.

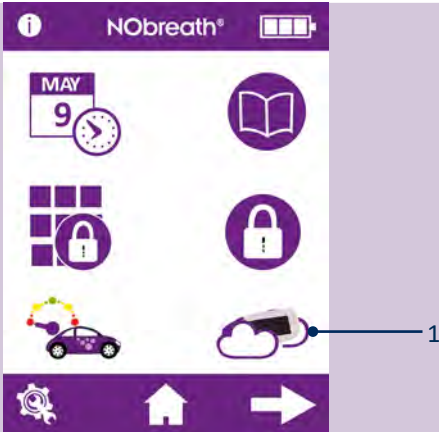

The NObreath® will begin sampling the atmosphere and an hourglass will be shown onscreen.




The result will be shown onscreen.


Press the back arrow (1) to return to the settings menu or the home icon (2) to return to the main screen.



### Adjusting the brightness of the display


To adjust the brightness of the display, go to the 2nd page of the settings menu and use the arrows to increase (1)/decrease (2) the brightness of the screen.

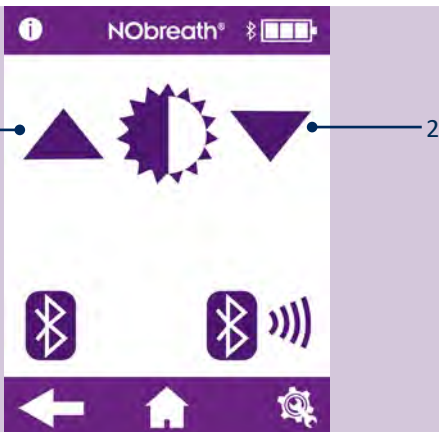

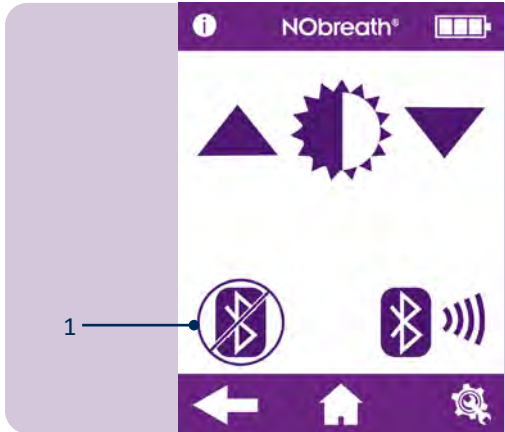

*Enable/disable Bluetooth®*


To enable Bluetooth®, go to the 2nd page of the settings menu and press the enable/disable Bluetooth® button (1).

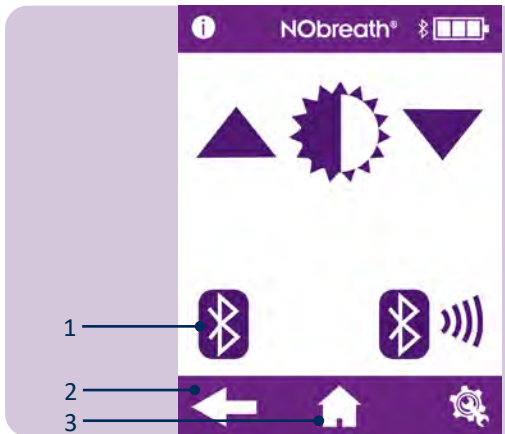

Once Bluetooth® is enabled, the Bluetooth® symbol will no longer be crossed out on the 2nd page of the settings menu and a Bluetooth® symbol will appear next to the battery status icon.

Press the icon (1) again to switch Bluetooth® off.

Press the back arrow (2) to return to the settings menu or the home icon (3) to return to the main screen.

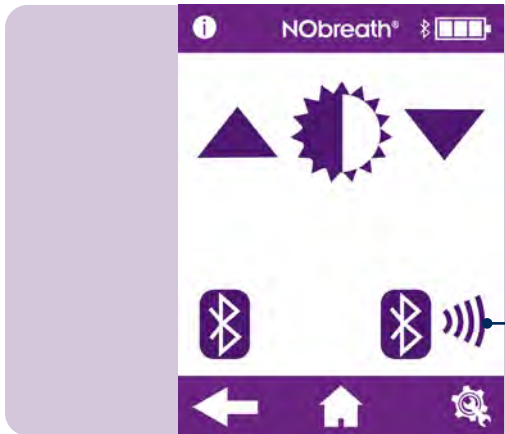

*Bluetooth® pairing*

To pair a device with the NObreath®, go to the 2nd page of the settings menu and press the Bluetooth® pairing icon (1).



The screen will display the Bluetooth® pairing PIN.


Please make sure the Bluetooth® on the NObreath® and the other device is switched on in order to pair with the NObreath®.

Press the back arrow (1) to return to the settings menu or the home icon (2) to return to the main screen.


## Data Reset



Using the screwdriver provided with the NObreath®, unscrew the screw on the back of the device.

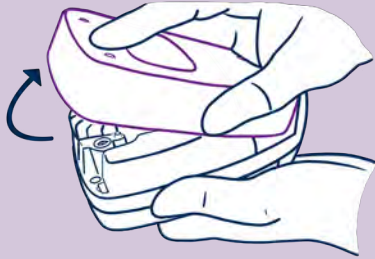

Remove the back cover by sliding and lifting it off.

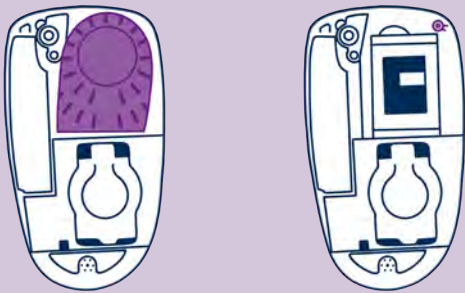

To access the Data Reset button, first remove the back cover and the breath drying cartridge.

This will reveal the Data Reset button at the top right of the NObreath®.



Press and hold the Data Reset button (1) for 5 seconds and the screen will reveal the reset icon.

**NOTE:** A data reset will erase all patient data from the device the PIN will be reset to the default, 0000.

Press the tick (2) to confirm the data reset or cross (3) to cancel.



An hourglass will display onscreen as the NObreath® begins erasing all data.

**NOTE:** *This can take up to 5 minutes to complete.*



Once complete, the screen will prompt for the back cover to be replaced.

Ensure that the breath drying cartridge has been re-inserted and then reattach the back cover.



All data will be erased and the home screen will display once more.

## Cybersecurity

**WARNING:** Precautions need to be taken when handling patient data, this should be completed by trained healthcare professionals only.

**CAUTION:** Security precautions need to be taken when connecting a NObreath<sup>®</sup> unit to a PC/laptop via USB or Wireless. Ensure the PC/laptop is in a secured environment (e.g. has a firewall and anti-virus software) in order to not expose the NObreath<sup>®</sup> to malwares.

**CAUTION:** The operating system of the PC/laptop should be kept up to date.

**WARNING:** Any data on the NObreath<sup>®</sup> device needs to be cleared (via a reset) before returning to Bedfont<sup>®</sup> or one of its distributors for service or repair and before the unit is disposed at end-of-life.

**WARNING:** The NObreath<sup>®</sup> needs to be stored in a secure place, e.g. a locked room or desk drawer/cupboard.

## Technical Specification

### *NObreath® device and dock*

Concentration range		5 – 500 ppb
Display		Full colour touchscreen
Detection principle		Electrochemical sensor
Repeatability		± 5ppb of measured value ≤ 50 ppb ± 10% of measured value > 50 ppb
Accuracy		± 5ppb of measured value ≤ 50 ppb ± 10% of measured value > 50 ppb
Power	NObreath® device	1 x main rechargeable Li-ion battery – Approx. 100 uses on fully charged battery Model: RRC1120. Voltage: 3.6 V / 3.7 V Capacity: 2350 mAh / 2000 mAh 2 x Li-ion coin cell batteries – Approx. 5 years Model: LIR2032/LIR2032H. Voltage: 3.7 V. Capacity: 45 mAh/70 mAh Model: LIR2450. Voltage: 3.7 V. Capacity: 120 mAh
	NObreath® Dock	Mains powered Input: 5 V, 0.5 A Output: 5 V, 0.5 A
	Plug	Input: 100 – 240 V ~ 50 / 60 Hz., 0.2 A Output: 5.0 V, 1.0 A
T90 response time		≤ 10 seconds
Temperature	Operating	59 - 86°F
	Storage/transport	32 - 122°F
	Calibration	21°C ± 4°C (17°C - 24°C) 70°F ± 7°F (63°F - 77°F)
Humidity	Operating	20 - 80% RH (non-condensing)
	Storage/transport	5 - 95% RH (non-condensing)
Operating/transport/storage Altitude		-1700 ft. to 6300 ft.
Operating/transport/storage pressure		800 – 1080 mbar
Expected sensor operating life		5 years (subject to servicing)
Limit of Detection		5 ppb
Sensor drift		< 5% per annum
Dimensions		Approx. 90 mm X 159 mm X 59 mm
Weight		Approx. 400 g
Materials	NObreath® device	Case: polycarbonate/ABS blend
	NObreath® Dock	Anti-microbial additive
Breath test time	Adult	12 seconds
	Child	10 seconds
	Ambient	30 seconds
Warm-up time		≤ 60 seconds
Maximum ambient operating level		350 ppb NO
CO cross interference		45 ppm ≤ 17.6 ppb

**NOTE:** Exhaled flow during FeNO measurement at 50 ml/sec ± 10% at 10 cm H<sub>2</sub>O.

### *NObreath® mouthpiece*

Infection control	An integrated infection control filter removes and traps > 99% of airborne bacteria and > 98% of viruses.
Dimensions	Approx. 180 mm X 25 mm X 15 mm
Weight	Approx. 11 g
Materials	Polypropylene

## Using the NObreath® with FeNOchart™

The NObreath® device is supplied with FeNOchart™ software, which allows patient data to be synchronised from the device to a computer, where results can be safely stored and analysed. FeNOchart™ can be downloaded directly from <https://www.nobreathfeno.com/fenochart/>

Insert the USB lead into the PC and connect the other end directly to the base of the NObreath® unit.



If using a Docking Station (where supplied) insert the USB lead into the PC and connect the other end to the rear of the docking station. Place the NObreath® into the docking station connecting to the micro USB in the base.



Before starting the software, ensure that the NObreath® is connected to the PC and switched on. Double click the FeNOchart™ icon on the PC to start the programme. Refer to the FeNOchart™ manual for how to operate the FeNOchart™ software.


## Buttons Explained



Information		Retry		Change PIN	
Adult test		Save		Disable PIN	
Child test		Next screen		Enable PIN	
Demo mode		Previous screen		Change flow meter style	
Patient profiles		Settings		Ambient test	
Home button		Date & time		Disable Bluetooth®	
Graph of results		Selected		Enable Bluetooth®	
Delete patient		Increase		Service Area (See service manual)	
Confirm		Decrease		Sensor calibration and NO scrubber reminder	
Cancel		Test log		Device full service reminder	
Sensor stabilising (device should be placed on charge)					



# Troubleshooting



Possible Cause		Recommended Action
 <p>Firmware v3.53</p>	 <p>Firmware v4.02 and above</p>	<p>The sensor requires calibrating or changing and the NO scrubber requires replacing within <math>\leq 30</math> days.</p> <p>The calibration or change of the sensor and the replacement of the NO scrubber is due by the date displayed onscreen.</p> <p>This reminder will be displayed every day until it has been reset by performing a sensor calibration or sensor change, and the NO scrubber has been replaced.</p>


Possible Cause		Recommended Action
 <p>Firmware v3.53</p>	 <p>Firmware v4.02 and above</p>	<p>The calibration or changing of the sensor and replacement of the NO scrubber is now due.</p> <p>The calibration or changing of the sensor and replacement of the NO scrubber was due on the date displayed.</p> <p>This reminder will be displayed every day until it has been reset by performing a sensor calibration or sensor change, and the NO scrubber has been replaced.</p>

Possible Cause		Recommended Action
 <p>Firmware v4.02 and above</p>	<p>The calibration or changing of the sensor and replacement of the NO scrubber is now overdue by <math>\geq 30</math> days.</p> <p>The date displayed is 365 days after the last sensor calibration or exchange.</p> <p>The calibration or changing of the sensor and replacement of the NO scrubber was due on the date displayed.</p> <p>This reminder will be displayed every day until it has been reset by performing a sensor calibration or sensor change, and the NO scrubber has been replaced.</p>	

 		Possible Cause	Recommended Action
		The NObreath® is due its full service in ≤ 30 days.	<p>The NObreath® is due its full service by the date displayed.</p> <p>A service reminder will be displayed every day until a full service has been carried out by a trained engineer.</p>

 		Possible Cause	Recommended Action
		<p>The NObreath® is now due its full service.</p> <p>5 years has elapsed since last full service.</p>	<p>The NObreath® was due its full service on the date displayed.</p> <p>A service reminder will be displayed every day until a full service has been carried out by a trained engineer.</p>

 		Possible Cause	Recommended Action
		The full service for the NObreath® is now overdue by ≥ 30 days.	<p>The full service for the NObreath® was due on the date displayed.</p> <p>A service reminder will be displayed every day until a full service has been carried out by a trained engineer.</p>


	Possible Cause	Recommended Action
	The sensor is stabilising after installation. The time displayed shows the time remaining until sensor has stabilised.	<p>The sensor requires 24 hours to stabilise; during this period, the NObreath® should be placed on charge.</p> <p>During this period, testing will not be possible. This screen will clear automatically after 24 hours.</p>

	<table border="1"> <thead> <tr> <th data-bbox="831 293 1155 344">Possible Cause</th> <th data-bbox="1155 293 1479 344">Recommended Action</th> </tr> </thead> <tbody> <tr> <td data-bbox="831 344 1155 696"> <p>There has been a sensor calibration error.</p> </td> <td data-bbox="1155 344 1479 696"> <p>Contact Bedfont® or their local distributor.</p> </td> </tr> </tbody> </table>	Possible Cause	Recommended Action	<p>There has been a sensor calibration error.</p>	<p>Contact Bedfont® or their local distributor.</p>
Possible Cause	Recommended Action				
<p>There has been a sensor calibration error.</p>	<p>Contact Bedfont® or their local distributor.</p>				


	<table border="1"> <thead> <tr> <th data-bbox="831 770 1155 822">Possible Cause</th> <th data-bbox="1155 770 1479 822">Recommended Action</th> </tr> </thead> <tbody> <tr> <td data-bbox="831 822 1155 1173"> <p>There has been a verification error in the flash memory of the device.</p> </td> <td data-bbox="1155 822 1479 1173"> <p>Contact Bedfont® or their local distributor.</p> </td> </tr> </tbody> </table>	Possible Cause	Recommended Action	<p>There has been a verification error in the flash memory of the device.</p>	<p>Contact Bedfont® or their local distributor.</p>
Possible Cause	Recommended Action				
<p>There has been a verification error in the flash memory of the device.</p>	<p>Contact Bedfont® or their local distributor.</p>				


	<table border="1"> <thead> <tr> <th data-bbox="831 1247 1155 1299">Possible Cause</th> <th data-bbox="1155 1247 1479 1299">Recommended Action</th> </tr> </thead> <tbody> <tr> <td data-bbox="831 1299 1155 1650"> <p>There has been an error in the NObreath® settings.</p> </td> <td data-bbox="1155 1299 1479 1650"> <p>Contact Bedfont® or their local distributor.</p> </td> </tr> </tbody> </table>	Possible Cause	Recommended Action	<p>There has been an error in the NObreath® settings.</p>	<p>Contact Bedfont® or their local distributor.</p>
Possible Cause	Recommended Action				
<p>There has been an error in the NObreath® settings.</p>	<p>Contact Bedfont® or their local distributor.</p>				

	<table border="1"> <thead> <tr> <th data-bbox="831 1722 1155 1774">Possible Cause</th> <th data-bbox="1155 1722 1479 1774">Recommended Action</th> </tr> </thead> <tbody> <tr> <td data-bbox="831 1774 1155 2125"> <p>There has been a failure in the flash memory of the device.</p> </td> <td data-bbox="1155 1774 1479 2125"> <p>Contact Bedfont® or their local distributor.</p> </td> </tr> </tbody> </table>	Possible Cause	Recommended Action	<p>There has been a failure in the flash memory of the device.</p>	<p>Contact Bedfont® or their local distributor.</p>
Possible Cause	Recommended Action				
<p>There has been a failure in the flash memory of the device.</p>	<p>Contact Bedfont® or their local distributor.</p>				

	<table border="1"> <thead> <tr> <th>Possible Cause</th> <th>Recommended Action</th> </tr> </thead> <tbody> <tr> <td>There has been a database failure.</td> <td>Contact Bedfont® or their local distributor.</td> </tr> </tbody> </table>	Possible Cause	Recommended Action	There has been a database failure.	Contact Bedfont® or their local distributor.
Possible Cause	Recommended Action				
There has been a database failure.	Contact Bedfont® or their local distributor.				

		<table border="1"> <thead> <tr> <th>Possible Cause</th> <th>Recommended Action</th> </tr> </thead> <tbody> <tr> <td>The back cover of the device is open.</td> <td>Make sure the back of the device is secure and the turn lock is closed.</td> </tr> <tr> <td>The back cover button is damaged, lost or stuck.</td> <td>Take the back cover off, check the back cover button is present. Replace back cover.</td> </tr> </tbody> </table>	Possible Cause	Recommended Action	The back cover of the device is open.	Make sure the back of the device is secure and the turn lock is closed.	The back cover button is damaged, lost or stuck.	Take the back cover off, check the back cover button is present. Replace back cover.
Possible Cause	Recommended Action							
The back cover of the device is open.	Make sure the back of the device is secure and the turn lock is closed.							
The back cover button is damaged, lost or stuck.	Take the back cover off, check the back cover button is present. Replace back cover.							

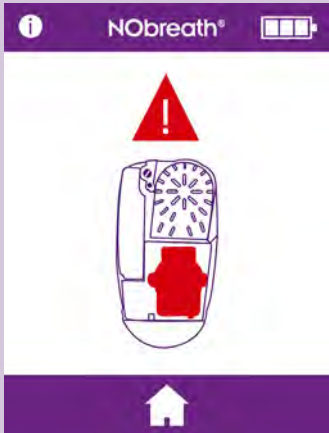	<table border="1"> <thead> <tr> <th>Possible Cause</th> <th>Recommended Action</th> </tr> </thead> <tbody> <tr> <td>No sensor detected.</td> <td>Ensure a sensor is inserted into the device.</td> </tr> <tr> <td>The sensor is not correctly inserted.</td> <td>Ensure the sensor is correctly inserted by pushing firmly in the top connector.</td> </tr> <tr> <td>Check the date and time. If this does not show the current date &amp; time the real time clock battery may be flat/empty.</td> <td>Change the date/time to the current date/time and charge the device battery fully.</td> </tr> <tr> <td>Sensor bias battery flat/empty.</td> <td>Charge the device battery fully. This will allow the sensor bias battery to also charge and re-bias the sensor. Instructions from the previous step may also have to be carried out.</td> </tr> <tr> <td>Sensor connector pins blocked.</td> <td>Remove the sensor and re-insert to clear any possible blockages.</td> </tr> </tbody> </table>	Possible Cause	Recommended Action	No sensor detected.	Ensure a sensor is inserted into the device.	The sensor is not correctly inserted.	Ensure the sensor is correctly inserted by pushing firmly in the top connector.	Check the date and time. If this does not show the current date & time the real time clock battery may be flat/empty.	Change the date/time to the current date/time and charge the device battery fully.	Sensor bias battery flat/empty.	Charge the device battery fully. This will allow the sensor bias battery to also charge and re-bias the sensor. Instructions from the previous step may also have to be carried out.	Sensor connector pins blocked.	Remove the sensor and re-insert to clear any possible blockages.
Possible Cause	Recommended Action												
No sensor detected.	Ensure a sensor is inserted into the device.												
The sensor is not correctly inserted.	Ensure the sensor is correctly inserted by pushing firmly in the top connector.												
Check the date and time. If this does not show the current date & time the real time clock battery may be flat/empty.	Change the date/time to the current date/time and charge the device battery fully.												
Sensor bias battery flat/empty.	Charge the device battery fully. This will allow the sensor bias battery to also charge and re-bias the sensor. Instructions from the previous step may also have to be carried out.												
Sensor connector pins blocked.	Remove the sensor and re-insert to clear any possible blockages.												




Possible Cause	Recommended Action
The device battery is flat/empty.	Plug the device directly into a power source, using the micro USB and power adapter or using the charging dock (where supplied). See “installation and setup” section of this manual.



The device does not switch on after being put on charge.

Possible Cause	Recommended Action
The device battery is flat/empty.	This is the muted charge mode. This screen will appear when the device has a depleted battery and is on charge. The device can charge for up to 90 minutes with a blank screen, and will not emit any sound during this time. If the device does not show any activity after 90 minutes, contact Bedfont® or the local distributor for assistance.

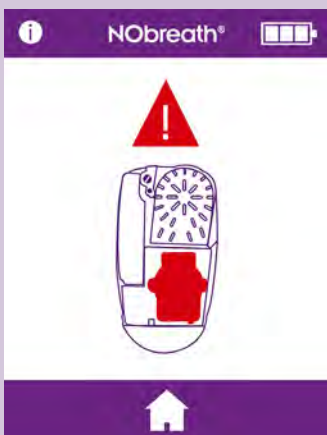


Suspicion that the device is giving erroneous/incorrect readings.


This image is an example only, and is not necessarily an example of an erroneous reading.

Possible Cause	Recommended Action
The device may be out of specification.	If the user suspects the device is giving erroneous readings, stop using it and check the accuracy by purchasing a CaliBag® from Bedfont® or the local distributor, or send to the local service centre.
The device may have been exposed to high levels of volatile organic compounds (VOC's) for example from cleaning agents.	Allow the device to rest for up to 24 hours in a VOC free environment.
The device may be showing testing in demo mode.	Ensure the breath test mode is being selected from the home screen.

*The device consistently reads 0 ppb*

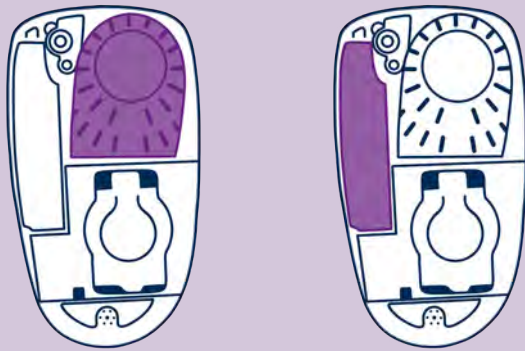

Possible Cause	Recommended Action
The drying cartridge is missing or disconnected.	Take the back cover off and check breath drying cartridge is present and fully located into the device. Replace the back cover.
The NO scrubber is missing or disconnected.	Take the back cover off and check NO scrubber is present and fully located into the device. Replace the back cover.

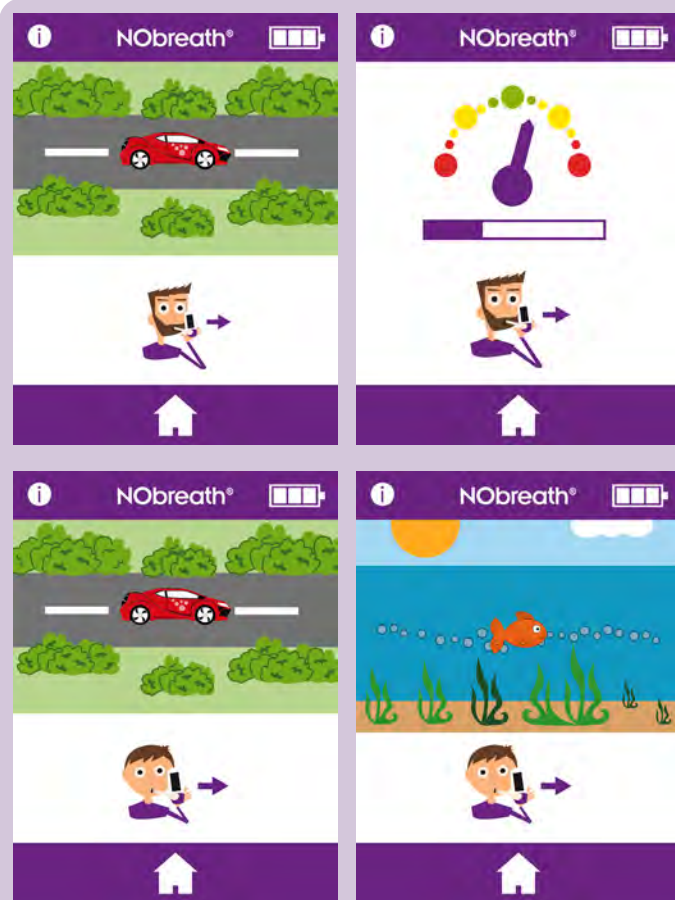















Possible Cause	Recommended Action
If the patient exhales outside of the exhalation guidelines, the test will beep before indicating a fail and a red cross will appear.	Press the retry icon to retake the test or if after multiple attempts the patient is unable to comply, the reading can be viewed by pressing the next arrow.



**WARNING:** Patients should exhale for the duration of time indicated by the device during a breath test. Failure to do so could impact the reading.

Notification Issue	Possible Cause	Recommended Action
<p>The device will not switch on</p>	The battery is missing.	Take the back cover off, check battery is present and fully located into the device. Replace back cover.
	The battery is flat.	Plug the device directly into a power source, using the micro USB and power adapter or using the charging dock (where supplied). See “Installation and Setup” section of this manual.
	The battery has been inserted incorrectly.	Contact Bedfont® or the local distributor for assistance.
	The device is not charging.	
	The battery contacts are blocked.	
	The power button is damaged.	
There is a screen issue.		
<p>The unit is reading incorrectly or showing 0 ppb</p>	The pump is not running.	The battery is low. Charge the device battery.
	The mouthpiece connection was loose during the test.	Ensure the mouthpiece is connected tightly.
	Check if any VOC's or alcohol based products have been used to wipe the device or mouthpiece.	Alcohol contaminations will affect the NO electro chemical sensor inside the device. Ensure no VOC's are used on the device and accessories related to the device.
	Check if any aerosols or room spray have been used where the device is used.	
	The vent holes are blocked.	Ensure vent holes are not blocked or covered by hands or something else during the test.
There are high levels of ambient NO.	Perform an ambient test as per the instructions. Levels should be ≤ 350 ppb, if levels are > 350 ppb, move to a different location and take a new measurement.	
<p>Rattling sound inside the unit</p>	This is from the scrubber material.	This is not an issue. Scrubber has potassium permanganate and charcoal buds inside the device to scrub ambient NO.
<p>NObreath® Dock is showing a red light</p>	Indicates a fault, overcurrent, undervoltage or overvoltage protection circuit has triggered.	Contact Bedfont® or the local distributor for assistance.

# Glossary of Symbols and Safety Information

Glossary of Symbols			
Title of Symbol	Symbol	Explanatory Text	Symbol and Standard References
Type BF Applied Part (Whole Device)		To identify a type BF applied part complying with IEC 60601-1	IEC 60417 – 5333 IEC 60601-1, Table D.1, Symbol 20
Degree of protection against ingress of liquid	IPX0 – not protected against water ingress	Degree of Ingress Protection Provided by Enclosure	IEC 60601-1, Table D.3, Symbol 2. IEC 60529
Consult instructions for use		Indicates the need for the user to consult the instructions for use	ISO 15223 – 1. Clause 5.4.3 ISO 7000 – 1641 IEC 60601-1, Table D.1, Symbol 11
Non-ionizing electromagnetic radiation  The device includes a Radio Frequency (RF) transmitter: Make: The device contains a Microchip Technology Inc. transmitter module. Module: Contains Transmitter Module FCC ID: T9J-RN42 / FCC ID: A8TBM78ABCDEFGH (Bluetooth®)		To indicate generally elevated, potentially hazardous, levels of non-ionizing radiation, or to indicate equipment or systems e.g. in the medical electrical area that include RF transmitters or that intentionally apply RF electromagnetic energy for diagnosis or treatment	IEC 60601-1-2 Clause 5.1.1 IEC 60417 - 5140
Direct current		To indicate on the rating plate that the equipment is suitable for direct current only; to identify relevant terminals	IEC 60601-1. Table D.1, Symbol 4
Dispose of according to WEEE		DO NOT THROW IN GENERAL RUBBISH DISPOSAL/TRASH! – Waste Electronic Equipment	EN 50419 Directive 2012/19/EU, Annex IX
Serial number		Indicates the manufacturers serial number so that a specific medical device can be identified	ISO 15223 – 1. Clause 5.1.7 ISO 7000 – 2498

<p><b>Manufactured by</b></p>		<p>Indicates the device manufacturer (*Note – Date of manufacture, name and address of manufacturer can be combined in one symbol)</p>	<p>ISO 15223 – 1. Clause 5.1.1 ISO 7000 – 3082</p>
<p><b>Manufacture date</b></p>		<p>Indicates the date when the medical device was manufactured</p>	<p>ISO 15223-1. Clause 5.1.3 ISO 7000 – 2497 FDA 21 CFR 801</p>
<p><b>Magnetic Resonance (MR) unsafe</b></p>		<p>3.1.14: An item which poses unacceptable risks to the patient, medical staff or other persons within the MR environment</p>	<p>ASTM F2503-20. Table 2, Symbol 7.3.3; 7.4.9.1; Fig.9</p>
<p><b>Caution</b></p>		<p>Indicates that caution is necessary when operating the device or control close to where the symbol is placed, or that the current situation needs operator awareness or operator action in order to avoid undesirable consequences</p>	<p>ISO 15223-1 Clause 5.4.4 ISO 7000 – 0434A FDA 21 CFR 801</p>
<p><b>Temperature limit</b></p>		<p>Indicates the temperature limits to which the medical device can be safely exposed</p>	<p>ISO 15223 – 1. Clause 5.3.7 ISO 7000 – 0632</p>
<p><b>Humidity limitation</b></p>		<p>Indicates the range of humidity to which the medical device can be safely exposed</p>	<p>ISO 15223 – 1. Clause 5.3.8 ISO 7000 – 2620</p>
<p><b>Atmospheric pressure limitation</b></p>		<p>Indicates the range of atmospheric pressure to which the medical device can be safely exposed</p>	<p>ISO 15223 – 1. Clause 5.3.9 ISO 7000 – 2621</p>
<p><b>General symbol for recovery/recyclable</b></p>		<p>To indicate that the marked item or its material is part of a recovery or recycling process</p>	<p>ISO 7000 – 1135</p>

Non-standard symbols			
Title of Symbol	Symbol	Explanatory Text	Symbol and Standard References
CE mark		Manufacturer's declaration of compliance to all relevant European Medical Device Regulations	Medical Device Regulation (EU) 2017/745.
Bedfont® logo		Manufacturer's logo	N/A
Type of protection against electric shock	Internally powered equipment	N/A	N/A
Degree of safety application in the presence of a flammable anaesthetic mixture with air, oxygen or nitrous oxide	Equipment not suitable for use in the presence of flammable mixtures.	N/A	N/A

## Wireless

This device contains a Microchip Technology Inc. transmitter module: Contains Transmitter Module FCC ID: T9J-RN42 / FCC ID: A8TBM78ABCDEFGH. This is in compliance with Part 15 of the FCC Rules, Spread Spectrum Transmitter.

Wireless Bluetooth® Low Energy (BLE) is used as a means of communication between the device and FeNOchart™ software running on a PC. The FeNOchart™ software is a charting program that retrospectively collects data from the NObreath® device when it is not monitoring. It is not time critical, there are no alarms.

Radio Technology: Bluetooth®: IEEE 802.15 Frequency-hopping spread spectrum.

Bluetooth® specification: v2.1 + EDR (Enhanced Data Rate) / V5.0.

Bluetooth® Class / Power: Class 2 Bluetooth® module. Software controllable power. Max power 4 dBm.

RF frequencies: 79 bands (1 MHz each; centered from 2.402 to 2.480 GHz) in the range 2,400- 2,483.5 GHz.

The Bluetooth® device is preconfigured with 128bit encryption and a CCITT CRC Checksum. There is no need or provision to change this setting.

The USB port is to be used for charging the NObreath® device, this should be carried out via the supplied USB lead and also can be used for transferring encrypted patient data to and from FeNOchart™ PC Software. The NObreath® is not intended to be connected to any wireless adaptors or any other USB Host.


## *Electromagnetic Immunity*

The NObreath® and NObreath® Dock comply with the IEC60601-1-2:2014 4th edition electromagnetic compatibility.

The NObreath® device is suitable for the electromagnetic environment of typical commercial or hospital settings.

During the immunity testing described below the NObreath® device continued to provide essential performance. We considered essential performance to be an NO reading within  $\pm 5$  ppb of inputted level. A deviation of  $\pm 5$  ppb has no physiological significance.

### **Warnings:**

- Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the NObreath® device, including cables specified by the manufacturer. Otherwise, degradation of the performance of this equipment could result.
- The NObreath® device should not be used adjacent to or stacked with other equipment. If adjacent or stacked use is necessary, the NObreath® device should be observed to verify normal operation. If operation is not normal, the NObreath® or the other equipment should be moved.
- Use of accessories, transducers and cables other than those specified or provided by the manufacturer of this equipment could result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment and result in improper operation.
- Avoid exposure to known sources of EMI (electromagnetic interference) such as Magnetic Resonance Imaging (MRI) systems, diathermy, lithotripsy, electrocautery, RFID (Radio Frequency Identification), and electromagnetic security systems such as metal detectors.
-  Keep the NObreath® outside the MRI scanner room.

Note that the presence of RFID devices may not be obvious. If such interference is suspected reorient equipment if possible, to maximize distances.

## Emissions

<p>The NObreath® device is intended for use in the electromagnetic environment specified below. The user should assure that it is used in such an environment.</p>		
Emission Tests	Compliance	Electromagnetic Environment – Guidance
<p>Conducted and Radiated RF Emissions CISPR 11</p>	<p>Group 1 Class A</p>	<p>The NObreath® device uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.</p>
<p>Conducted and Radiated RF Emissions CISPR 11</p>	<p>Group 1 Class A</p>	<p>The NObreath® device is suitable for use in all establishments other than domestic, and may be used in domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes, provided the following warning is heeded:</p> <p><b>WARNING:</b> This equipment/system is intended for use by healthcare professionals only. This equipment/system may cause radio interference or may disrupt the operation of nearby equipment. It may be necessary to take mitigation measures, such as re-orienting or relocating the NObreath® device or shielding the location.</p>

**NOTE:** *The EMISSIONS characteristics of this equipment make it suitable for use in industrial areas and hospitals (CISPR 11 class A). If it is used in a residential environment (for which CISPR 11 class B is normally required) this equipment might not offer adequate protection to radio-frequency communication services. The user might need to take mitigation measures, such as relocating or re-orienting the equipment.*

## Immunity

<b>Guidance and manufacturer’s declaration: Electromagnetic immunity</b>			
The NObreath® is intended for use in the electromagnetic environment specified below. The customer or the user of the NObreath® should ensure that it is used in such an environment.			
<b>Immunity test</b>	<b>IEC 60601 test level</b>	<b>Compliance level</b>	<b>Electromagnetic environment guidance</b>
Electrostatic Discharge (ESD) IEC 61000-4-2	± 8 kV contact ± 2, 4, 8 and 15 kV air	± 8 kV contact ± 2, 4, 8 and 15 kV air	Floor should be wood, concrete or ceramic floor tile. If floors are covered with synthetic material the relative humidity should be at least 30%.
Electrical fast transient/ bursts (immunity) IEC 61000-4-4	± 2 kV	± 2 kV	Mains power quality should be that of a typical commercial or hospital environment.
Surge (immunity) IEC 61000-4-5	± 0.5, 1.0 kV L-L ± 0.5, 1.0, 2.0 kV L-E	± 0.5, 1.0 kV L-L ± 0.5, 1.0, 2.0 kV L-E	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	100% 0.01 Seconds 100% 0.02 Seconds 30% 0.5 Seconds 100% 5 Seconds	100% 0.01 Seconds 100% 0.02 Seconds 30% 0.5 Seconds 100% 5 Seconds	Mains power quality should be that of a typical commercial or hospital environment. If the user of the NObreath® requires continued operation during power mains interruptions beyond that provided by the battery, it is recommended that the NObreath® is powered from an uninterruptible power supply.
Power frequency (50/60Hz) Magnetic field IEC 61000-4-8	30 A/m	30 A/m	Power frequency magnetic fields should be at levels characteristic of a typical commercial or hospital environment.

<b>Electromagnetic Immunity</b>		
The NObreath® is intended for use in the electromagnetic environment specified below. The customer or the user of the NObreath® should assure that it is used in such an environment.		
<b>Immunity Test</b>	<b>Compliance Level</b>	<b>Electromagnetic Environment – Guidance</b>
Conducted RF IEC 61000-4-6 Radiated RF IEC 61000-4-3	3 Vrms (1 kHz 80%) 150 kHz – 80 MHz 3 V/m (1 kHz 80%) 80 MHz – 2.7 GHz	The NObreath® is suitable for the electromagnetic environment of typical commercial or hospital settings.

NObreath® has also been tested for immunity to RF wireless communications equipment as below.

Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment guidance
Radiated RF IEC 61000-4-3	385 MHz 27 V/m 450 MHz 28 V/m 710 MHz 9 V/m 745 MHz 9 V/m 780 MHz 9 V/m 810 MHz 28 V/m 870 MHz 28 V/m 930 MHz 28 V/m 1720 MHz 28 V/m 1845 MHz 28 V/m 1970 MHz 28 V/m 2450 MHz 28 V/m 5240 MHz 9 V/m 5500 MHz 9 V/m 5785 MHz 9 V/m	385 MHz 27 V/m 450 MHz 28 V/m 710 MHz 9 V/m 745 MHz 9 V/m 780 MHz 9 V/m 810 MHz 28 V/m 870 MHz 28 V/m 930 MHz 28 V/m 1720 MHz 28 V/m 1845 MHz 28 V/m 1970 MHz 28 V/m 2450 MHz 28 V/m 5240 MHz 9 V/m 5500 MHz 9 V/m 5785 MHz 9 V/m	The NObreath® device is suitable for the electromagnetic environment of typical commercial or hospital settings.

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy, and if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

## Summary of the clinical data

### Study 1: A clinical Precision study comparing intra and inter usability of FeNO measurement using the NObreath®.

In one of the studies conducted, the clinical precision, as it relates to user bias of the NObreath®, was evaluated in a mixed study population of 76 participants - including 24 paediatric participants (ages 7 - 17 years) and 52 adults (18 years +). Participants were asked to obtain 2 NObreath® measurements with the assistance of 3 health care professionals (HCPs), for a total of 6 NObreath® evaluations per participant. The clinical precision study was designed to capture the accuracy and precision of the NObreath® device, therefore FeNO values acquired by subjects covered potential FeNO values which would be observed in clinical practice. The within subject precision\* was assessed from this study population and is presented in the table below:

Median Concentrations	N	Within Subject Mean SD (ppb)	Within Subject Mean CV (%)	95% CI for CV (%)
0 to < 10	10	0.8034172	13.35%	7.85%; 18.85%
10 to < 20	21	1.2430966	9.18%	6.73%; 11.64%
20 to < 30	23	0.9720727	4.17%	2.48%; 5.85%
30 to < 40	5	1.2279205	3.65%	1.3%; 6%
40 to < 50	5	1.3867462	3.17%	0.23%; 6.1%
>= 50	12	1.4078969	1.89%	1.29%; 2.48%

\*3 subjects in the clinical precision study had a large variation between the measurements. 1 subject was from median concentration bin of >= 50 ppb and 2 subjects were from the median concentration bin of 40 to < 50 ppb. The %CV for these subjects was 10.24%, 21.54%, and 14.17%. This table excludes data from these three subjects.

There were no adverse events, serious injuries, issues or problems with use of the NObreath® in participants.

### Study 2: A clinical study illustrating asthma patient response to anti-inflammatory therapy using the NObreath®.

A second study also evaluated the clinical efficacy of the NObreath®; A total of 186 patients (n= 95 18+ and n=91 7 to 17 years of age) participated in a longitudinal study where measurements for FeNO, spirometry, and asthma control questionnaires were completed at baseline (Visit 1) and two weeks later (Visit 2) after therapeutic agents were administered. For those with elevated initial FeNO defined by ATS > 25 ppb for adults and > 20 ppb for children (total n=139), there was a fall in mean FeNO measured by NObreath® in patients with elevated FeNO levels for combined adult and paediatric treatment population (n=139). Results showed a mean change of -13.7 ppb (-27.7%) with a mean SD of 17.8.

#### The Decline in FeNO was accompanied by the following changes in subjective and objective asthma measures.

The following secondary outcome measures showed the following after 2 weeks of corticosteroid therapy that accompanied the fall in FeNO described above.

ACQ:  
Mean ACQ score fell by -29.7% after corticosteroids.

FEV1:  
There was a mean FEV1 change of 10.1% after corticosteroids.

**References:**

1. An Official ATS Clinical Practice Guideline: Interpretation of Exhaled Nitric Oxide Levels (FeNO) for Clinical Applications | American Journal of Respiratory and Critical Care Medicine [Internet]. Atsjournals.org. 2021 [cited 21 July 2021]. Available from: <https://www.atsjournals.org/doi/full/10.1164/rccm.9120-11ST>
2. Asthma Control Questionnaire (ACQ) [Internet]. Thoracic.org. 2021 [cited 21 July 2021]. Available from: <https://www.thoracic.org/members/assemblies/assemblies/srn/questionnaires/acq.php>
3. Minimal Clinically Important Differences in Pharmacological Trials [Internet]. Atsjournals.org. 2021 [cited 21 July 2021]. Available from: [https://www.atsjournals.org/doi/pdf/10.1164/rccm.201310-1863PP#:~:text=Lung%20Function%20\(FEV1\)&text=The%20American%20Thoracic%20Society%2FEuropean,not%20clinically%20important%20\(8\)1863PP#:~:text=Lung%20Function%20\(FEV1\)&text=The%20American%20Thoracic%20Society%2FEuropean,not%20clinically%20important%20\(8\)](https://www.atsjournals.org/doi/pdf/10.1164/rccm.201310-1863PP#:~:text=Lung%20Function%20(FEV1)&text=The%20American%20Thoracic%20Society%2FEuropean,not%20clinically%20important%20(8)1863PP#:~:text=Lung%20Function%20(FEV1)&text=The%20American%20Thoracic%20Society%2FEuropean,not%20clinically%20important%20(8))

## Analytical Performance Data

### Linearity

Four NObreath® devices were tested as part of a linearity study. 2 devices were tested in ‘adult mode’ and 2 devices were tested in ‘child mode’. Nitric oxide was mixed in a balance gas of air to produce NO concentration levels between < 5 and > 500 ppb. The results are listed in the table below.

Device	Mode (child or adult)	Slope	y-intercept	R <sup>2</sup>
1	Adult	0.9751	1.8037	0.9993
2	Adult	1.0199	-1.8566	0.9997
3	Child	1.0092	-0.6022	0.9992
4	Child	1.0308	1.0465	0.9999

### Precision/ Reproducibility and Accuracy

#### Precision/ Reproducibility

The repeatability and within-device precision was analysed using samples across a range of 10, 25, 75, 200, 350 & 500 ppb concentrations. The measurements were performed over 5 days, 2 sessions per day, 2 measurements per session across 15 separate devices.

Repeatability is an estimation of variation within 1 test run in 1 day. Within-device precision is an estimate of variation between test runs and days.

NObreath®’s precision/reproducibility is claimed to be a standard deviation of ≤ 5 ppb for readings ≤ 50 ppb and a CV of ≤ 10% for readings > 50 ppb. The precision/reproducibility testing performed confirmed that the precision/reproducibility performance of the NObreath® fell within these specifications.

**Limit of Detection**

The limit of detection was determined based on CLSI EP17-A2. Ten devices were tested at 3 ppb (50 replicates) and 5 ppb (50 replicates) over three days in both child and adult modes. Nitric oxide samples were mixed in a balance gas of simulated breath. The limit of detection was calculated using the parametric option in CLSI EP17-A2, using the following formulas:  $LoB = \mu_B + 1.645 \sigma_B$  and  $LoD = LoB + 1.645 \sigma_S$ . The results of the limit of detection analysis support the claimed detection limit of 5 ppb. The results are presented in the below two tables.

N= 50  
 $LoB = \mu_B + 1.645 \sigma_B$   
 $LoB = \mu_B + 1.645 \sigma_S$

	ADULT	
	3	5
Mean	3.42	5.42
SD	0.475094	0.4686063
95th	1.645	1.645
LoB	4.2015296	6.1908573
LoD	4.9830592	6.9617146
95% CI	0.13169	0.12989
95% CI -	3.29	5.29
95% CI +	3.55	5.55

At the nominal value of 3 ppb, the overall mean measured value was 3.42 ppb (95% CI 3.29;3.55). At the nominal value of 5 ppb, the overall mean measured value was 5.42 ppb (95% CI 5.29;5.55) which supports the claimed detection limit of 5 ppb in adult mode.

N= 50  
 $LoB = \mu_B + 1.645 \sigma_B$   
 $LoB = \mu_B + 1.645 \sigma_S$

	CHILD	
	3	5
Mean	3.63	5.47
SD	0.4997183	0.5347553
95th	1.645	1.645
LoB	4.4480366	6.3456725
LoD	5.2700732	7.225345
95% CI	0.13851	0.14822
95% CI -	3.49	5.32
95% CI +	3.76	5.61

At the nominal value of 3 ppb, the overall mean measured value was 3.61 ppb (95% CI 3.49;3.76). At the nominal value of 5 ppb, the overall mean measured value was 5.47 ppb (95% CI 5.32;5.61) which supports the claimed detection limit of 5 ppb in child mode.

**Interpretation of FeNO Values**

For interpretation of FeNO values, please refer to the ATS Clinical Practice Guideline at <https://www.thoracic.org/statements/resources/allergy-asthma/feno-document.pdf>

## Warranty

Bedfont® Scientific Limited warrants the NObreath® device and sensors, batteries excepted, to be free of defects in materials and workmanship for a period of 5 years from the date of shipment, subject to service and maintenance requirements.

Bedfont's sole obligation under this warranty is limited to repairing or replacing, at its choice, any item covered under this warranty when such an item is returned intact and prepaid, to Bedfont® or the local representative.



This warranty is automatically invalidated if the products are altered or tampered with by unauthorised personnel, or have been subject to misuse, neglect or accident. At the end of the product's life, contact Bedfont® or its distributor for disposal instructions.

Single-patient use consumables and accessories should be disposed of in line with local clinical waste guidelines.

Never dispose of any electronic instrument or batteries in domestic waste. At the end of the product's life, contact Bedfont® or its distributor for disposal instructions.

## Vigilance

As a medical device manufacturer, Bedfont® Scientific Ltd. must have a vigilance system in place to report any adverse incidents which have been caused by its medical products.

An adverse event is identified by meeting all three of the following criteria:

- An event has occurred; typical events include, but are not limited to:
  - A malfunction or deterioration in the characteristics or performance.
- The Manufacturer's device is suspected to be a contributory cause of the incident.
- The event led, or might have led to one of the following outcomes:
  - **Death of patient, USER or other person.**
  - **Serious deterioration in the state of health of a patient, USER or other person.**
- Manufacturers of medical devices must report an adverse event in the following timescales:
  - **Serious public health threat:** Immediately.
  - **Death or unanticipated serious deterioration in state of health:** Immediately, (without any delay that could not be justified) but not later than 10 elapsed calendar days following the date of awareness of the event.
  - **Others:** Immediately (without any delay that could not be justified) but not later than 15 elapsed calendar days following awareness of the event (UK reporting time frame is 15 days).

Any of Bedfont® Scientific Ltd. users who experience an adverse event relating to a product which meets the above criteria must immediately report this to Bedfont® and the National Competent Authority of which the country where the incident occurred.

Please contact Bedfont® Scientific Ltd. with all relevant information on:

Email: [ask@bedfont.com](mailto:ask@bedfont.com)

Telephone: 0044 1622 851122

## Returns

Please contact Bedfont® or its local distributor for instructions on returning goods.

## Responsible Manufacturer and Contacts

**Bedfont® Scientific Ltd.**  
Station Yard, Station Road,  
Harrietsham,  
Maidstone, Kent,  
ME17 1JA  
United Kingdom

[www.bedfont.com](http://www.bedfont.com)  
[www.nobreathfeno.com](http://www.nobreathfeno.com)

[ask@bedfont.com](mailto:ask@bedfont.com)  
0044 1622 851122



### USA Representative for Sales, Service & Support:

coVita  
3200 Research Forest Drive Suite A1  
The Woodlands, TX 77381  
Tel: 800.707.5751 Fax: 800.721.2377  
Email: [service@covita.net](mailto:service@covita.net) Website: [www.covita.net](http://www.covita.net)





**bedfont**<sup>®</sup>  
est. 1976



Official Bedfont Distributor

**USA Representative for Sales, Service & Support:**

coVita

3200 Research Forest Drive Suite A1

The Woodlands, TX 77381

Tel: 800.707.5751 Fax: 800.721.2377

Email: [service@covita.net](mailto:service@covita.net) Website: [www.covita.net](http://www.covita.net)



***World leaders in breath analysis.***



Bedfont<sup>®</sup> Scientific Ltd.  
Station Road, Harrietsham, Maidstone,  
Kent, ME17 1JA England  
Tel: +44 (0)1622 851122 Fax: +44 (0)1622 854860  
Email: [ask@bedfont.com](mailto:ask@bedfont.com) Web: [www.bedfont.com](http://www.bedfont.com)

EC

REP

Emergo Europe B.V.  
Westervoortsedijk 60  
6827 AT Arnhem  
The Netherlands.

© Bedfont<sup>®</sup> Scientific Limited 2025

Issue 24 - October 2025, Part No: LAB759\_USA

Bedfont<sup>®</sup> Scientific Limited reserves the right to change or update this literature without prior notice.

Registered in: England and Wales. Registered No: 1289798



MD 502905